

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051079.D
 Acq On : 03 Oct 2022 13:56
 Operator : JC/MD
 Sample : VU1003WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK195

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051079.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	95	rVB	222807	256632	15.44%	2.115%
2	1.912	170	178	196	rBV	222787	291704	17.55%	2.404%
3	2.565	368	381	400	rBV	336980	540522	32.52%	4.455%
4	2.690	417	420	424	rBV3	535	488	0.03%	0.004%
5	2.790	447	451	455	rVV4	803	746	0.04%	0.006%
6	2.899	483	485	490	rVB3	824	616	0.04%	0.005%
7	2.935	494	496	500	rVB2	547	289	0.02%	0.002%
8	3.044	521	530	541	rVB3	8576	15040	0.90%	0.124%
9	3.186	556	574	590	rBV2	11758	27186	1.64%	0.224%
10	3.247	590	593	598	rVB	378	327	0.02%	0.003%
11	3.272	598	601	604	rBV	598	383	0.02%	0.003%
12	3.292	605	607	611	rVB	443	281	0.02%	0.002%
13	3.369	627	631	634	rBV3	408	411	0.02%	0.003%
14	3.514	673	676	680	rBV2	406	334	0.02%	0.003%
15	3.629	707	712	718	rBV2	409	514	0.03%	0.004%
16	3.745	744	748	750	rBV2	377	285	0.02%	0.002%
17	3.854	780	782	785	rBV	435	292	0.02%	0.002%
18	3.874	785	788	795	rVB	660	560	0.03%	0.005%
19	3.915	795	801	806	rVB2	730	713	0.04%	0.006%
20	3.941	806	809	812	rBV	506	287	0.02%	0.002%
21	4.025	829	835	837	rBV2	324	316	0.02%	0.003%
22	4.112	860	862	866	rVB	669	347	0.02%	0.003%
23	4.198	885	889	890	rBV	501	306	0.02%	0.003%
24	4.279	911	914	920	rVB2	483	417	0.03%	0.003%
25	4.497	979	982	987	rVB	461	307	0.02%	0.003%
26	4.629	1010	1023	1063	rBV	148003	427468	25.72%	3.523%
27	4.909	1107	1110	1119	rVB4	629	822	0.05%	0.007%
28	5.063	1140	1158	1184	rBV	306322	673146	40.50%	5.548%
29	5.160	1184	1188	1191	rBV2	671	520	0.03%	0.004%
30	5.288	1221	1228	1237	rVB6	1114	1858	0.11%	0.015%
31	5.362	1247	1251	1252	rBV2	573	384	0.02%	0.003%
32	5.427	1268	1271	1274	rBV2	509	319	0.02%	0.003%
33	5.456	1274	1280	1287	rVB2	573	741	0.04%	0.006%
34	5.497	1287	1293	1298	rBV2	450	542	0.03%	0.004%
35	5.726	1339	1364	1394	rBV2	615345	1661911	100.00%	13.698%
36	5.928	1425	1427	1431	rVB3	837	516	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051079.D
 Acq On : 03 Oct 2022 13:56
 Operator : JC/MD
 Sample : VU1003WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK195

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	5.967	1437	1439	1442	rVB3	630	341	0.02%	0.003%
38	5.983	1442	1444	1448	rVB4	577	365	0.02%	0.003%
39	6.041	1459	1462	1467	rBV2	802	598	0.04%	0.005%
40	6.105	1477	1482	1484	rBV3	627	575	0.03%	0.005%
41	6.192	1504	1509	1512	rBV	258	258	0.02%	0.002%
42	6.247	1512	1526	1560	rBV	479095	920532	55.39%	7.587%
43	6.362	1560	1562	1565	rBV3	923	585	0.04%	0.005%
44	6.491	1598	1602	1603	rBV3	413	259	0.02%	0.002%
45	6.529	1603	1614	1627	rVB3	15679	29784	1.79%	0.245%
46	6.591	1627	1633	1637	rBV5	807	981	0.06%	0.008%
47	6.690	1648	1664	1687	rBV	393528	773142	46.52%	6.372%
48	6.864	1716	1718	1722	rVB2	766	480	0.03%	0.004%
49	7.195	1813	1821	1824	rBV4	1111	1495	0.09%	0.012%
50	7.336	1859	1865	1869	rBV	408	378	0.02%	0.003%
51	7.491	1908	1913	1915	rBV2	362	323	0.02%	0.003%
52	7.565	1923	1936	1954	rBV	187124	339984	20.46%	2.802%
53	7.729	1985	1987	1991	rBV	613	469	0.03%	0.004%
54	7.774	1998	2001	2004	rBV2	535	357	0.02%	0.003%
55	7.845	2020	2023	2025	rBV	416	314	0.02%	0.003%
56	7.896	2025	2039	2064	rBV	698322	1206970	72.63%	9.948%
57	8.179	2115	2127	2144	rBV	138977	239014	14.38%	1.970%
58	8.375	2185	2188	2190	rBV	747	514	0.03%	0.004%
59	8.455	2210	2213	2216	rBV	379	278	0.02%	0.002%
60	8.475	2216	2219	2223	rVV	490	382	0.02%	0.003%
61	8.555	2238	2244	2252	rVB4	1177	1489	0.09%	0.012%
62	8.639	2257	2270	2304	rBV2	359440	863072	51.93%	7.114%
63	8.806	2321	2322	2326	rVB4	1160	559	0.03%	0.005%
64	8.909	2352	2354	2355	rBV4	618	318	0.02%	0.003%
65	8.970	2370	2373	2378	rVV2	524	371	0.02%	0.003%
66	8.996	2378	2381	2384	rVB2	555	418	0.03%	0.003%
67	9.025	2387	2390	2394	rBV4	366	315	0.02%	0.003%
68	9.076	2402	2406	2410	rVB2	367	326	0.02%	0.003%
69	9.118	2416	2419	2422	rBV2	381	259	0.02%	0.002%
70	9.214	2444	2449	2450	rBV2	306	253	0.02%	0.002%
71	9.262	2458	2464	2467	rVB2	300	349	0.02%	0.003%
72	9.417	2496	2512	2534	rBV	693399	1170909	70.46%	9.651%
73	9.607	2567	2571	2575	rBV2	595	522	0.03%	0.004%
74	9.626	2575	2577	2579	rVV2	581	286	0.02%	0.002%
75	9.642	2579	2582	2589	rVB3	708	895	0.05%	0.007%
76	9.693	2594	2598	2605	rVB3	645	801	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051079.D
 Acq On : 03 Oct 2022 13:56
 Operator : JC/MD
 Sample : VU1003WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK195

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	9.725	2605	2608	2611	rBV2	393	274	0.02%	0.002%
78	10.005	2686	2695	2700	rBV2	627	994	0.06%	0.008%
79	10.060	2708	2712	2716	rBV2	438	480	0.03%	0.004%
80	10.169	2744	2746	2751	rVB3	348	284	0.02%	0.002%
81	10.468	2835	2839	2842	rBV2	566	488	0.03%	0.004%
82	10.513	2850	2853	2857	rVB2	569	340	0.02%	0.003%
83	10.552	2862	2865	2868	rBV2	428	317	0.02%	0.003%
84	10.587	2872	2876	2878	rBV	393	320	0.02%	0.003%
85	10.690	2903	2908	2913	rBV	513	633	0.04%	0.005%
86	10.754	2915	2928	2947	rBV	536648	881937	53.07%	7.269%
87	10.877	2964	2966	2971	rVB3	582	456	0.03%	0.004%
88	10.970	2991	2995	2997	rBV2	493	400	0.02%	0.003%
89	11.134	3044	3046	3050	rVB	573	349	0.02%	0.003%
90	11.529	3166	3169	3172	rBV	517	316	0.02%	0.003%
91	11.812	3244	3257	3275	rBV	523812	839836	50.53%	6.922%
92	12.098	3344	3346	3349	rVB2	546	274	0.02%	0.002%
93	12.118	3349	3352	3357	rBV2	785	820	0.05%	0.007%
94	12.192	3362	3375	3399	rBV	579251	933873	56.19%	7.697%
95	12.410	3440	3443	3445	rBV2	578	390	0.02%	0.003%
96	12.642	3512	3515	3517	rBV	591	400	0.02%	0.003%
97	12.854	3578	3581	3586	rBV3	623	712	0.04%	0.006%
98	13.201	3686	3689	3695	rBV3	726	858	0.05%	0.007%
99	13.558	3798	3800	3803	rBV2	531	312	0.02%	0.003%
100	15.166	4298	4300	4307	rBV3	894	741	0.04%	0.006%




Sum of corrected areas: 12132854

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051079.D
Acq On : 03 Oct 2022 13:56
Operator : JC/MD
Sample : VU1003WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK195

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

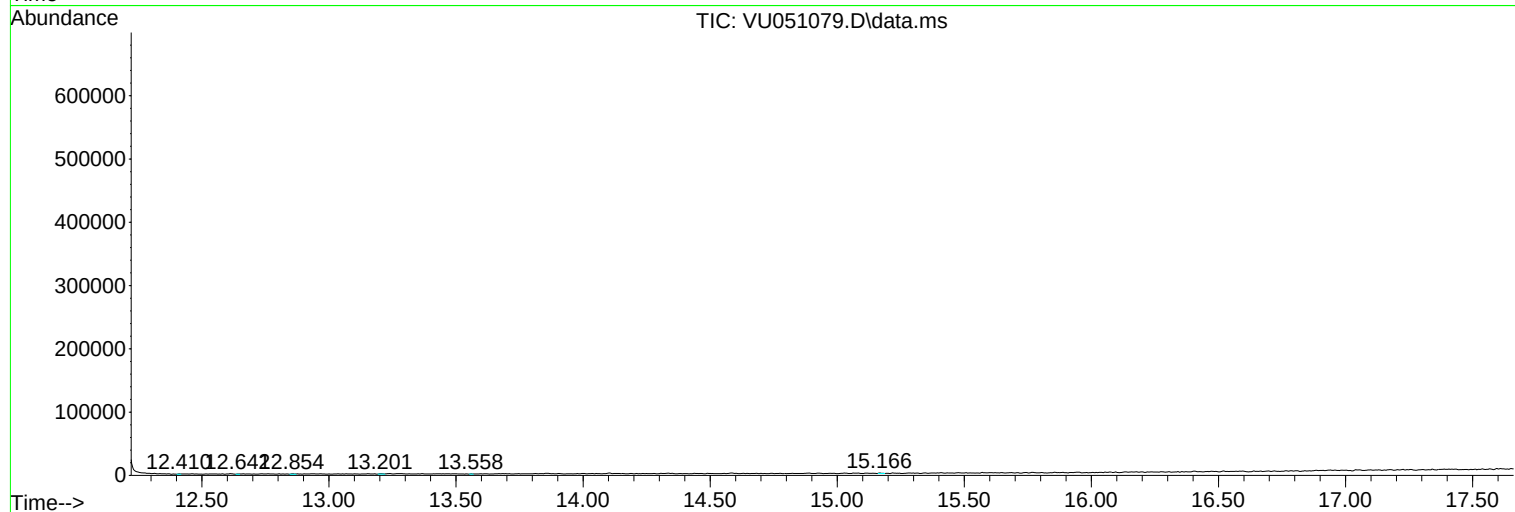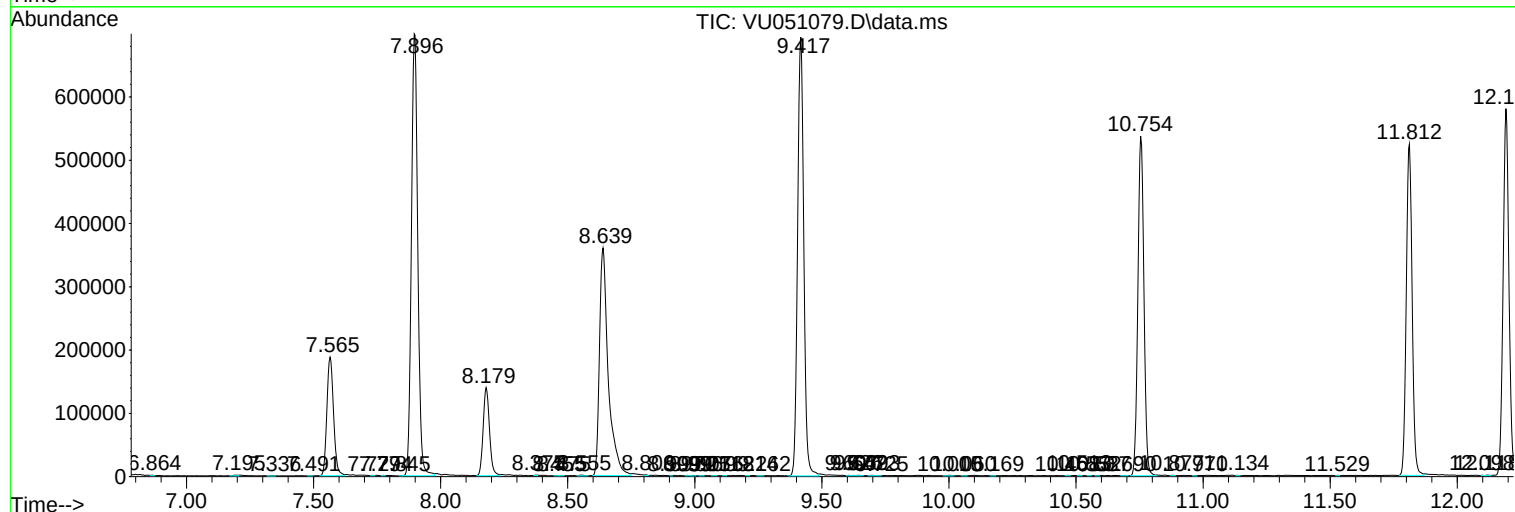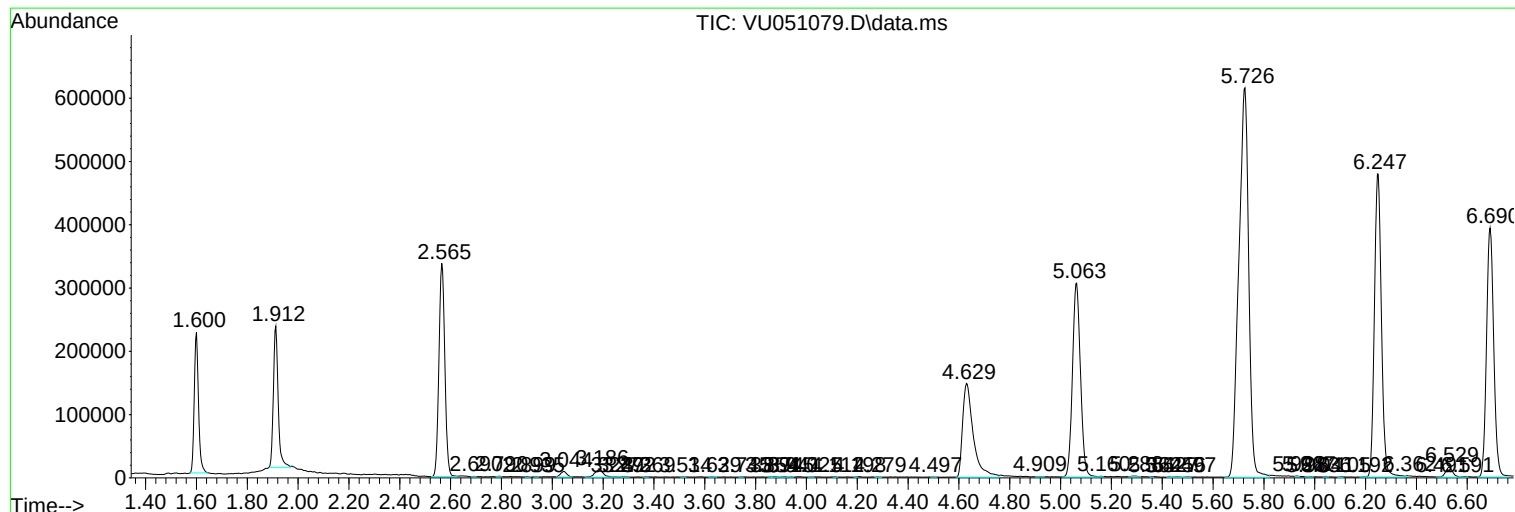

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051079.D
Acq On : 03 Oct 2022 13:56
Operator : JC/MD
Sample : VU1003WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK195

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051079.D
Acq On : 03 Oct 2022 13:56
Operator : JC/MD
Sample : VU1003WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK195

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc