

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051080.D
 Acq On : 03 Oct 2022 14:19
 Operator : JC/MD
 Sample : N4859-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051080.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	99	rVB	253637	301139	15.40%	2.175%
2	1.906	169	176	192	rVB	225705	301796	15.43%	2.180%
3	2.565	369	381	395	rBV	392972	634689	32.46%	4.585%
4	2.633	397	402	415	rVB2	6719	11067	0.57%	0.080%
5	2.732	431	433	437	rBV2	552	284	0.01%	0.002%
6	2.880	476	479	485	rVB3	995	691	0.04%	0.005%
7	3.044	523	530	540	rVB5	1775	2981	0.15%	0.022%
8	3.189	565	575	585	rBV6	1957	3833	0.20%	0.028%
9	3.334	616	620	622	rBV2	414	291	0.01%	0.002%
10	3.356	622	627	628	rVV2	444	348	0.02%	0.003%
11	3.549	682	687	689	rBV	299	297	0.02%	0.002%
12	3.600	700	703	707	rVB2	392	308	0.02%	0.002%
13	3.629	707	712	714	rBV	419	324	0.02%	0.002%
14	3.645	714	717	721	rVB2	459	312	0.02%	0.002%
15	3.668	721	724	729	rVB	514	386	0.02%	0.003%
16	3.703	732	735	741	rBV2	398	392	0.02%	0.003%
17	3.748	745	749	755	rBV	476	568	0.03%	0.004%
18	3.996	822	826	828	rVV2	459	365	0.02%	0.003%
19	4.009	828	830	837	rVV3	546	490	0.03%	0.004%
20	4.073	844	850	853	rBV2	442	450	0.02%	0.003%
21	4.092	853	856	861	rVB	518	339	0.02%	0.002%
22	4.137	864	870	874	rBV	602	633	0.03%	0.005%
23	4.237	898	901	905	rBV2	560	432	0.02%	0.003%
24	4.292	915	918	923	rVB2	315	276	0.01%	0.002%
25	4.433	958	962	965	rVV2	534	477	0.02%	0.003%
26	4.623	1007	1021	1054	rBV	185986	494560	25.29%	3.573%
27	4.899	1104	1107	1110	rVB2	506	336	0.02%	0.002%
28	4.922	1110	1114	1117	rBV3	597	506	0.03%	0.004%
29	5.063	1140	1158	1185	rBV3	386283	1003888	51.34%	7.252%
30	5.288	1225	1228	1229	rBV	649	393	0.02%	0.003%
31	5.324	1237	1239	1244	rVB4	554	401	0.02%	0.003%
32	5.372	1249	1254	1256	rBV3	588	461	0.02%	0.003%
33	5.417	1265	1268	1272	rBV2	410	302	0.02%	0.002%
34	5.555	1308	1311	1315	rBV	403	289	0.01%	0.002%
35	5.600	1321	1325	1330	rVB2	509	497	0.03%	0.004%
36	5.723	1342	1363	1394	rBV2	721608	1955544	100.00%	14.127%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051080.D
 Acq On : 03 Oct 2022 14:19
 Operator : JC/MD
 Sample : N4859-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.128	1487	1489	1495	rVB2	608	508	0.03%	0.004%
38	6.182	1502	1506	1511	rVB3	642	649	0.03%	0.005%
39	6.247	1511	1526	1548	rBV	470780	904241	46.24%	6.532%
40	6.526	1602	1613	1626	rVV3	22962	42373	2.17%	0.306%
41	6.575	1626	1628	1633	rVB2	1177	759	0.04%	0.005%
42	6.616	1639	1641	1645	rBV3	472	383	0.02%	0.003%
43	6.690	1649	1664	1690	rBV	464769	912540	46.66%	6.592%
44	6.890	1724	1726	1730	rVB3	602	307	0.02%	0.002%
45	6.935	1738	1740	1743	rBV	360	295	0.02%	0.002%
46	6.989	1751	1757	1759	rBV2	381	386	0.02%	0.003%
47	7.105	1779	1793	1804	rBV2	11049	19940	1.02%	0.144%
48	7.192	1812	1820	1830	rVB6	1645	2855	0.15%	0.021%
49	7.314	1855	1858	1863	rBV2	393	465	0.02%	0.003%
50	7.430	1892	1894	1901	rVB	317	296	0.02%	0.002%
51	7.565	1923	1936	1957	rBV	225145	400772	20.49%	2.895%
52	7.829	2015	2018	2023	rVB2	810	709	0.04%	0.005%
53	7.896	2023	2039	2055	rBV	817200	1399972	71.59%	10.114%
54	8.073	2091	2094	2096	rBV2	561	440	0.02%	0.003%
55	8.118	2106	2108	2111	rBV2	528	307	0.02%	0.002%
56	8.179	2114	2127	2149	rBV	159999	281692	14.40%	2.035%
57	8.314	2166	2169	2171	rBV	593	375	0.02%	0.003%
58	8.404	2194	2197	2200	rVB2	697	435	0.02%	0.003%
59	8.423	2200	2203	2205	rBV2	601	443	0.02%	0.003%
60	8.555	2238	2244	2248	rVB6	1265	1405	0.07%	0.010%
61	8.636	2255	2269	2305	rBV3	455894	1055273	53.96%	7.624%
62	8.899	2348	2351	2353	rBV3	729	393	0.02%	0.003%
63	9.021	2386	2389	2391	rBV3	472	300	0.02%	0.002%
64	9.076	2405	2406	2411	rVB	561	332	0.02%	0.002%
65	9.105	2411	2415	2418	rBV	587	462	0.02%	0.003%
66	9.121	2418	2420	2424	rVB	529	321	0.02%	0.002%
67	9.153	2424	2430	2432	rBV2	567	537	0.03%	0.004%
68	9.205	2442	2446	2450	rBV2	409	419	0.02%	0.003%
69	9.417	2498	2512	2538	rBV	690495	1152799	58.95%	8.328%
70	9.568	2556	2559	2566	rVB4	1677	1824	0.09%	0.013%
71	9.603	2568	2570	2573	rVB	654	365	0.02%	0.003%
72	9.645	2581	2583	2587	rVB2	423	277	0.01%	0.002%
73	9.693	2592	2598	2606	rVB4	2559	3477	0.18%	0.025%
74	9.848	2644	2646	2649	rBV2	449	296	0.02%	0.002%
75	9.970	2678	2684	2688	rBV2	394	584	0.03%	0.004%
76	10.057	2706	2711	2716	rBV2	604	638	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051080.D
 Acq On : 03 Oct 2022 14:19
 Operator : JC/MD
 Sample : N4859-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.099	2718	2724	2725	rBV	873	677	0.03%	0.005%
78	10.375	2808	2810	2816	rBV2	405	405	0.02%	0.003%
79	10.497	2842	2848	2852	rVV2	513	612	0.03%	0.004%
80	10.552	2863	2865	2871	rVB2	485	312	0.02%	0.002%
81	10.754	2915	2928	2954	rBV	642772	1032414	52.79%	7.458%
82	10.883	2964	2968	2973	rBV4	793	834	0.04%	0.006%
83	10.954	2987	2990	2994	rBV3	400	307	0.02%	0.002%
84	11.031	3010	3014	3018	rBV3	474	399	0.02%	0.003%
85	11.099	3029	3035	3037	rBV3	630	576	0.03%	0.004%
86	11.160	3051	3054	3058	rVB3	679	461	0.02%	0.003%
87	11.690	3216	3219	3225	rVB2	429	484	0.02%	0.003%
88	11.809	3244	3256	3279	rBV	512038	817064	41.78%	5.903%
89	11.992	3312	3313	3320	rBV3	433	383	0.02%	0.003%
90	12.192	3361	3375	3392	rBV	653982	1070604	54.75%	7.734%
91	12.475	3461	3463	3466	rBV	634	466	0.02%	0.003%
92	12.578	3493	3495	3500	rBV2	508	503	0.03%	0.004%
93	13.012	3627	3630	3634	rBV2	670	517	0.03%	0.004%
94	13.635	3821	3824	3827	rBV2	671	488	0.02%	0.004%
95	13.860	3891	3894	3897	rBV3	907	624	0.03%	0.005%
96	14.185	3993	3995	3999	rBV2	589	551	0.03%	0.004%
97	14.237	4008	4011	4014	rBV3	766	668	0.03%	0.005%
98	14.269	4018	4021	4025	rBV	740	714	0.04%	0.005%
99	14.414	4063	4066	4070	rBV2	808	592	0.03%	0.004%
100	14.732	4162	4165	4170	rBV4	674	488	0.02%	0.004%




Sum of corrected areas: 13842332

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051080.D
Acq On : 03 Oct 2022 14:19
Operator : JC/MD
Sample : N4859-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

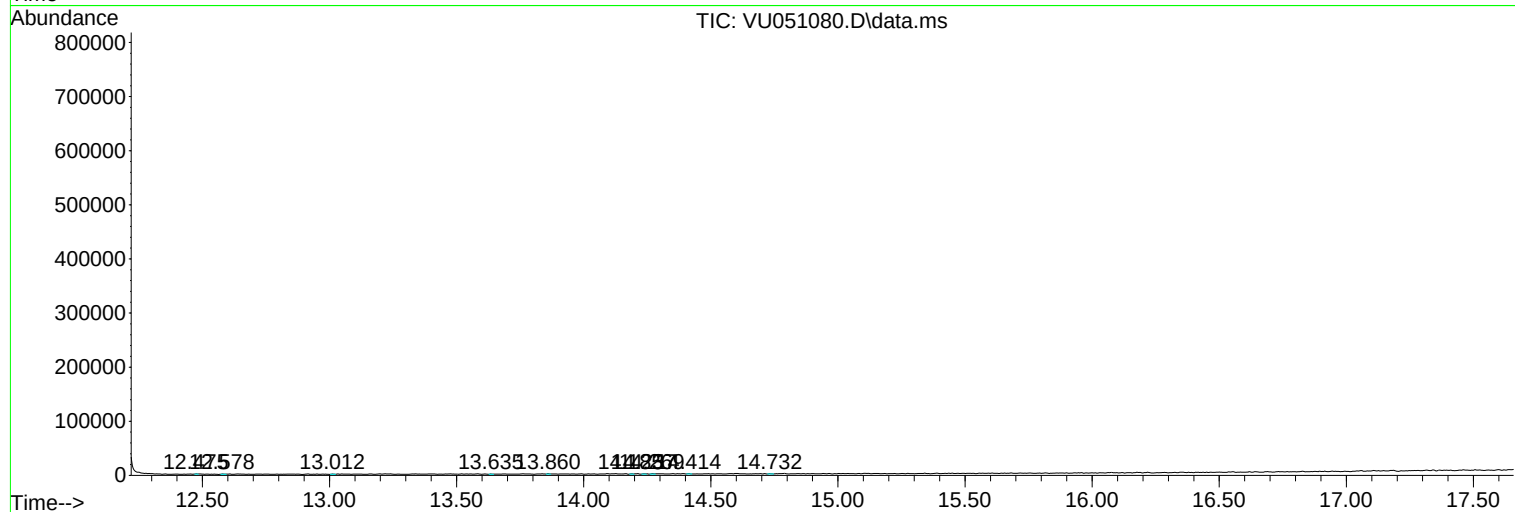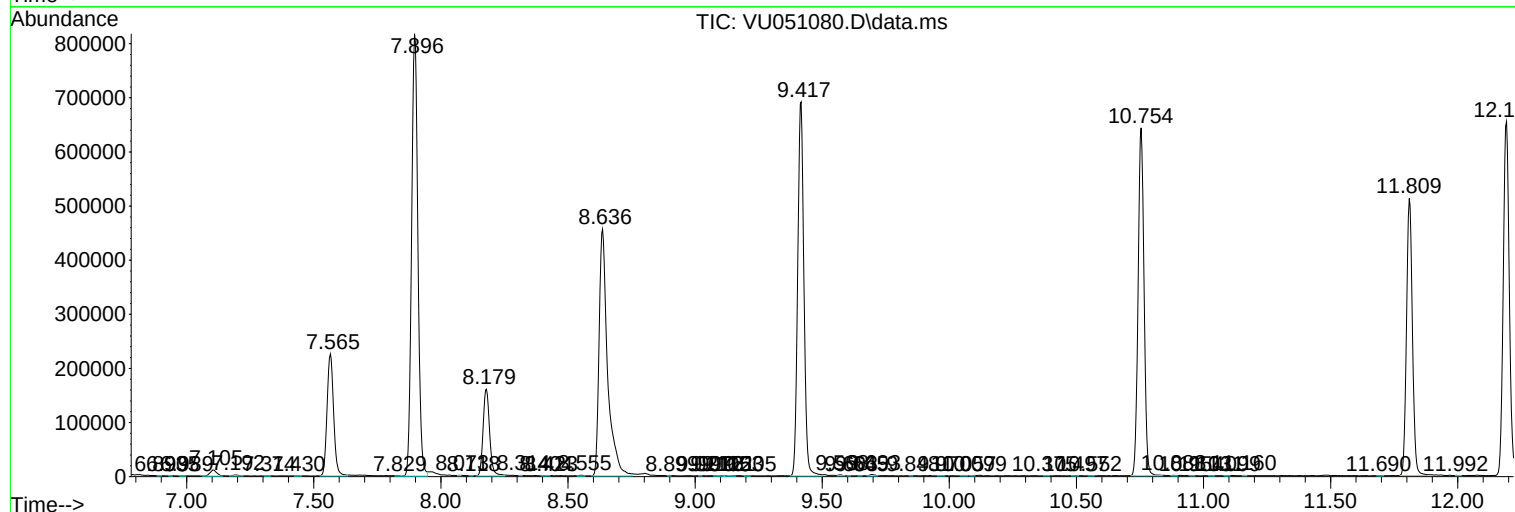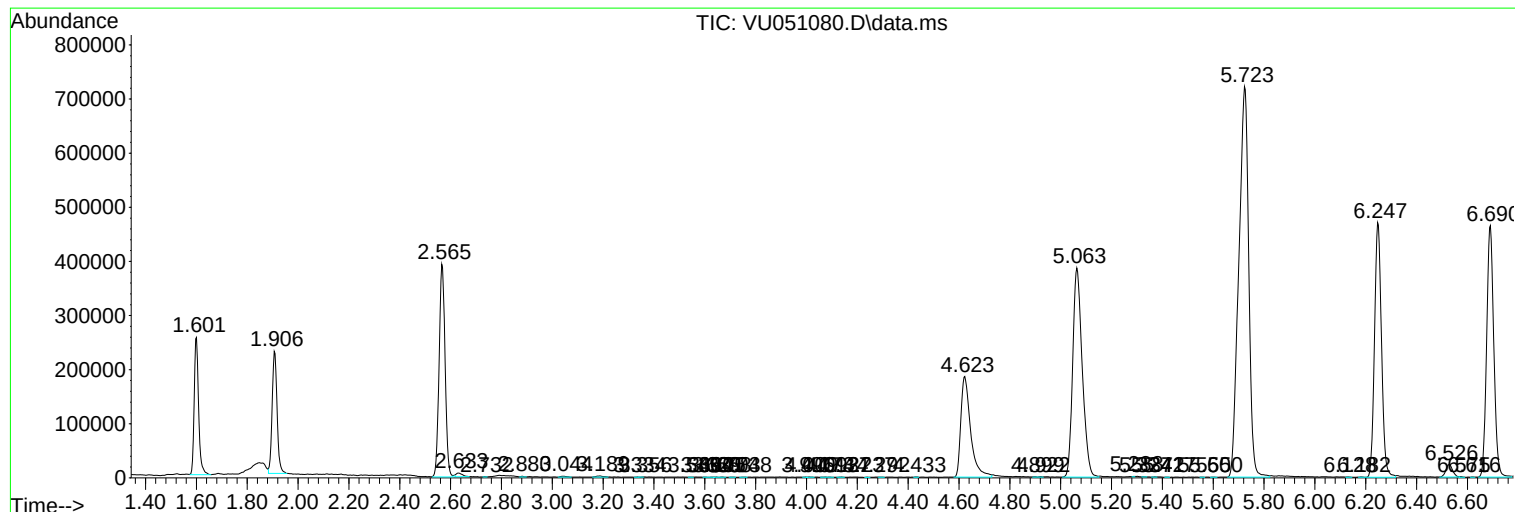

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051080.D
Acq On : 03 Oct 2022 14:19
Operator : JC/MD
Sample : N4859-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051080.D
Acq On : 03 Oct 2022 14:19
Operator : JC/MD
Sample : N4859-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc