

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051084.D
 Acq On : 03 Oct 2022 15:56
 Operator : JC/MD
 Sample : N4869-12DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J37DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	211095	253036	15.19%	1.945%
2	1.906	169	176	195	rVB	206634	277976	16.68%	2.137%
3	2.565	368	381	396	rBV	336730	542389	32.55%	4.170%
4	2.713	421	427	429	rBV3	694	676	0.04%	0.005%
5	2.742	431	436	443	rVV4	930	1419	0.09%	0.011%
6	3.044	520	530	541	rVB3	7660	14059	0.84%	0.108%
7	3.186	559	574	587	rBV2	13227	30672	1.84%	0.236%
8	3.363	618	629	641	rVV6	3247	6540	0.39%	0.050%
9	3.446	651	655	658	rBV	666	496	0.03%	0.004%
10	3.478	661	665	667	rVV2	366	349	0.02%	0.003%
11	3.504	670	673	677	rVV2	521	438	0.03%	0.003%
12	3.556	686	689	694	rVV	349	331	0.02%	0.003%
13	3.629	710	712	719	rBV2	327	293	0.02%	0.002%
14	3.716	736	739	746	rVB2	453	469	0.03%	0.004%
15	3.752	746	750	754	rBV2	314	302	0.02%	0.002%
16	3.777	754	758	763	rBV2	532	545	0.03%	0.004%
17	3.935	804	807	811	rBV2	290	301	0.02%	0.002%
18	3.980	818	821	825	rBV	469	447	0.03%	0.003%
19	4.105	855	860	864	rVB2	506	469	0.03%	0.004%
20	4.128	864	867	874	rVB2	410	501	0.03%	0.004%
21	4.173	875	881	883	rBV2	329	292	0.02%	0.002%
22	4.395	946	950	952	rBV2	563	419	0.03%	0.003%
23	4.465	968	972	978	rVB2	325	337	0.02%	0.003%
24	4.494	978	981	985	rVB2	459	403	0.02%	0.003%
25	4.623	1008	1021	1058	rBV	158857	437129	26.24%	3.361%
26	4.964	1123	1127	1134	rBV	601	735	0.04%	0.006%
27	4.993	1134	1136	1141	rVB4	449	346	0.02%	0.003%
28	5.060	1141	1157	1181	rBV	307976	682516	40.97%	5.248%
29	5.218	1203	1206	1209	rVB4	817	524	0.03%	0.004%
30	5.369	1249	1253	1255	rBV	658	435	0.03%	0.003%
31	5.385	1255	1258	1264	rVB2	623	609	0.04%	0.005%
32	5.459	1277	1281	1287	rBV2	642	712	0.04%	0.005%
33	5.555	1308	1311	1315	rVB	470	355	0.02%	0.003%
34	5.588	1315	1321	1326	rVB2	341	385	0.02%	0.003%
35	5.723	1340	1363	1390	rBV2	618293	1666080	100.00%	12.810%
36	6.051	1463	1465	1469	rVB2	588	322	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051084.D
 Acq On : 03 Oct 2022 15:56
 Operator : JC/MD
 Sample : N4869-12DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J37DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.112	1479	1484	1485	rBV2	418	299	0.02%	0.002%
38	6.125	1485	1488	1491	rVV3	599	440	0.03%	0.003%
39	6.154	1491	1497	1500	rVV2	196	284	0.02%	0.002%
40	6.247	1511	1526	1553	rBV	465144	892599	53.57%	6.863%
41	6.536	1603	1616	1628	rVV7	19446	42700	2.56%	0.328%
42	6.690	1648	1664	1684	rBV	399787	784686	47.10%	6.033%
43	6.893	1725	1727	1730	rVB3	670	390	0.02%	0.003%
44	6.912	1730	1733	1736	rVB2	474	309	0.02%	0.002%
45	7.031	1766	1770	1772	rBV	378	325	0.02%	0.002%
46	7.121	1794	1798	1804	rVV	689	963	0.06%	0.007%
47	7.163	1807	1811	1813	rVV2	396	354	0.02%	0.003%
48	7.195	1813	1821	1828	rVB7	1522	2746	0.16%	0.021%
49	7.244	1828	1836	1844	rBV2	333	568	0.03%	0.004%
50	7.469	1899	1906	1909	rVB2	352	360	0.02%	0.003%
51	7.498	1909	1915	1919	rBV2	404	402	0.02%	0.003%
52	7.565	1923	1936	1958	rBV	194736	342783	20.57%	2.636%
53	7.684	1970	1973	1975	rBV4	738	513	0.03%	0.004%
54	7.777	1996	2002	2006	rBV3	342	499	0.03%	0.004%
55	7.809	2006	2012	2015	rBV4	273	303	0.02%	0.002%
56	7.896	2025	2039	2060	rBV	691589	1197163	71.86%	9.205%
57	8.073	2092	2094	2100	rBV3	507	383	0.02%	0.003%
58	8.179	2115	2127	2143	rVV2	132927	228848	13.74%	1.760%
59	8.330	2171	2174	2180	rBV3	560	359	0.02%	0.003%
60	8.420	2196	2202	2204	rBV3	524	472	0.03%	0.004%
61	8.456	2210	2213	2215	rBV2	599	444	0.03%	0.003%
62	8.491	2222	2224	2230	rVB4	540	432	0.03%	0.003%
63	8.552	2230	2243	2257	rBV	581503	988079	59.31%	7.597%
64	8.636	2257	2269	2301	rVB4	375824	864775	51.90%	6.649%
65	8.967	2365	2372	2376	rBV4	613	694	0.04%	0.005%
66	8.989	2376	2379	2383	rBV2	345	296	0.02%	0.002%
67	9.038	2390	2394	2399	rVB3	572	547	0.03%	0.004%
68	9.092	2409	2411	2415	rBV2	609	459	0.03%	0.004%
69	9.417	2498	2512	2543	rBV	674861	1131928	67.94%	8.703%
70	9.697	2595	2599	2605	rVB3	655	586	0.04%	0.005%
71	9.803	2629	2632	2635	rBV2	487	357	0.02%	0.003%
72	9.870	2648	2653	2655	rBV2	357	335	0.02%	0.003%
73	9.941	2669	2675	2676	rBV2	340	344	0.02%	0.003%
74	9.993	2687	2691	2694	rBV3	506	477	0.03%	0.004%
75	10.038	2702	2705	2713	rVB2	374	467	0.03%	0.004%
76	10.076	2714	2717	2720	rVV	346	313	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051084.D
 Acq On : 03 Oct 2022 15:56
 Operator : JC/MD
 Sample : N4869-12DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J37DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.099	2722	2724	2731	rVB2	618	528	0.03%	0.004%
78	10.176	2742	2748	2751	rBV2	448	433	0.03%	0.003%
79	10.372	2803	2809	2812	rBV	559	591	0.04%	0.005%
80	10.468	2833	2839	2841	rBV	587	610	0.04%	0.005%
81	10.488	2842	2845	2850	rVV	679	774	0.05%	0.006%
82	10.523	2854	2856	2864	rVV2	458	460	0.03%	0.004%
83	10.584	2871	2875	2877	rBV3	498	422	0.03%	0.003%
84	10.755	2915	2928	2953	rBV	550455	892092	53.54%	6.859%
85	10.886	2967	2969	2975	rVB3	559	336	0.02%	0.003%
86	11.025	3009	3012	3016	rBV2	568	332	0.02%	0.003%
87	11.076	3024	3028	3034	rBV3	467	454	0.03%	0.003%
88	11.436	3134	3140	3146	rVB2	520	651	0.04%	0.005%
89	11.484	3150	3155	3157	rBV	279	285	0.02%	0.002%
90	11.584	3182	3186	3191	rBV2	285	320	0.02%	0.002%
91	11.620	3195	3197	3201	rVV2	369	282	0.02%	0.002%
92	11.809	3243	3256	3284	rBV	490132	783205	47.01%	6.022%
93	12.076	3336	3339	3341	rBV2	563	367	0.02%	0.003%
94	12.118	3349	3352	3355	rBV3	550	411	0.02%	0.003%
95	12.192	3362	3375	3401	rBV	546364	909242	54.57%	6.991%
96	12.562	3487	3490	3494	rBV2	469	324	0.02%	0.002%
97	12.931	3602	3605	3609	rBV3	536	528	0.03%	0.004%
98	13.169	3676	3679	3681	rBV2	430	295	0.02%	0.002%
99	13.719	3847	3850	3852	rBV2	497	342	0.02%	0.003%
100	13.880	3897	3900	3901	rBV	593	375	0.02%	0.003%




Sum of corrected areas: 13006247

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051084.D
Acq On : 03 Oct 2022 15:56
Operator : JC/MD
Sample : N4869-12DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J37DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

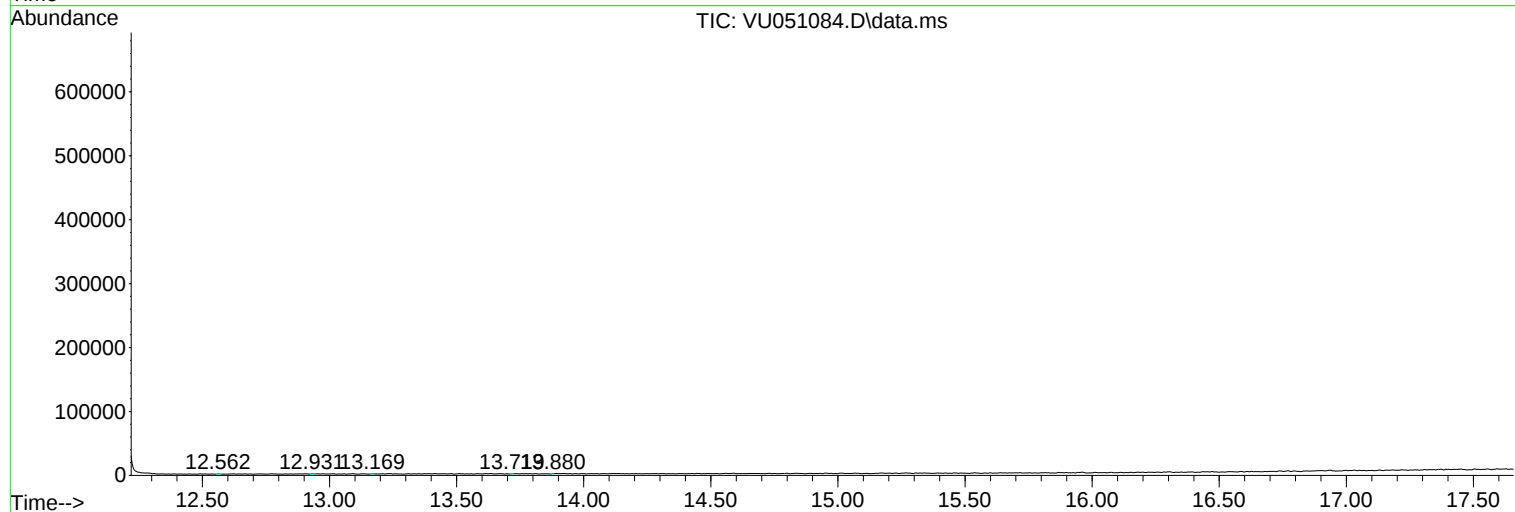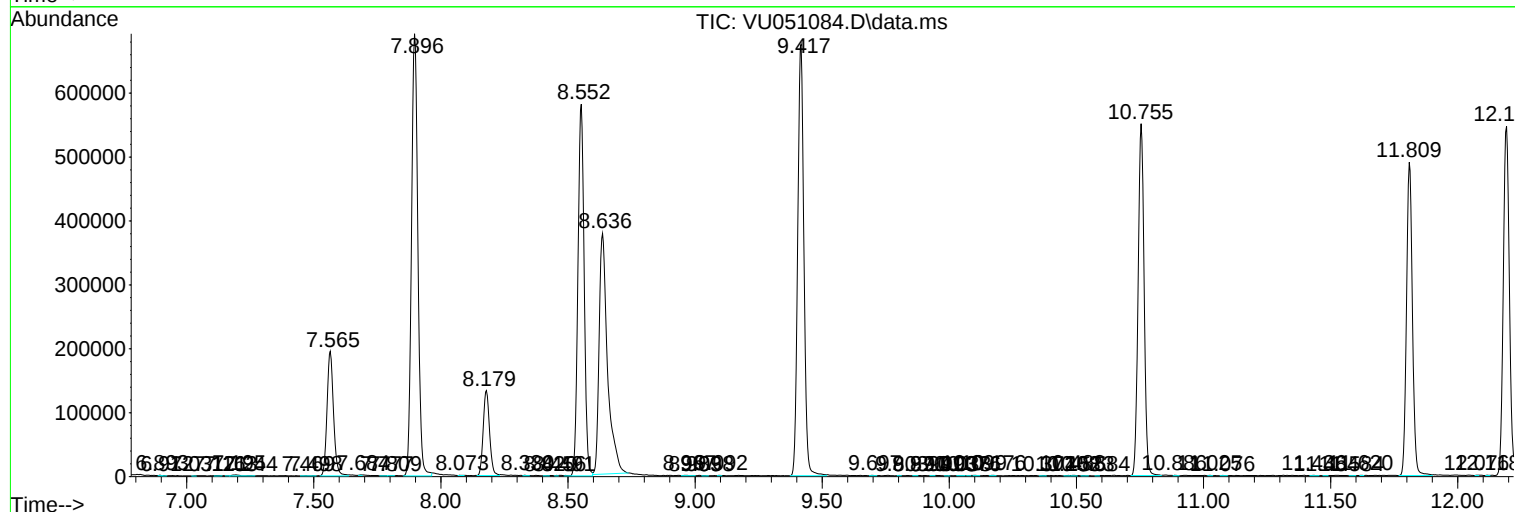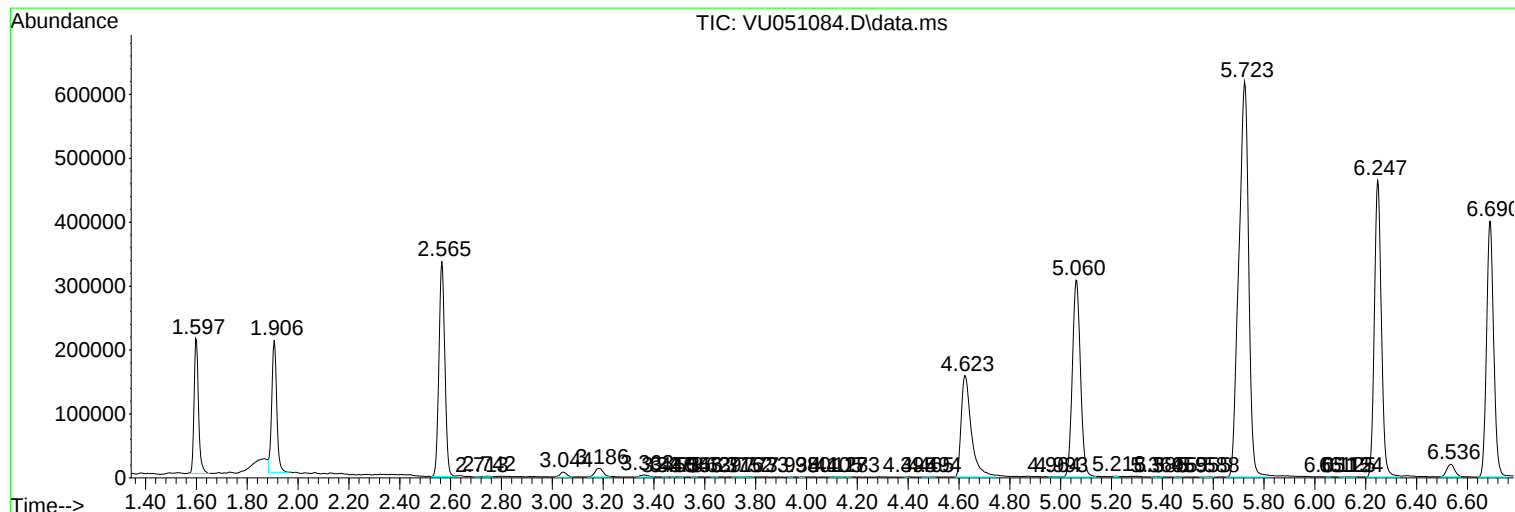

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051084.D
Acq On : 03 Oct 2022 15:56
Operator : JC/MD
Sample : N4869-12DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J37DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051084.D
Acq On : 03 Oct 2022 15:56
Operator : JC/MD
Sample : N4869-12DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J37DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------