

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051085.D
 Acq On : 03 Oct 2022 16:19
 Operator : JC/MD
 Sample : N4869-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J00DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	100	rBV	216614	261392	15.43%	1.906%
2	1.906	168	176	198	rVB	194705	260758	15.39%	1.902%
3	2.517	364	366	369	rBV	575	348	0.02%	0.003%
4	2.565	369	381	397	rBV	342542	553002	32.64%	4.033%
5	2.790	446	451	459	rVB5	599	928	0.05%	0.007%
6	2.938	493	497	500	rBV2	508	500	0.03%	0.004%
7	3.044	521	530	542	rBV	8740	15113	0.89%	0.110%
8	3.186	559	574	589	rBV	13644	30454	1.80%	0.222%
9	3.292	603	607	610	rBV	377	317	0.02%	0.002%
10	3.327	615	618	621	rBV	440	330	0.02%	0.002%
11	3.353	621	626	631	rBV4	720	874	0.05%	0.006%
12	3.488	662	668	671	rBV	386	329	0.02%	0.002%
13	3.623	706	710	713	rBV	479	468	0.03%	0.003%
14	3.642	714	716	720	rVV2	401	344	0.02%	0.003%
15	3.729	738	743	745	rVV2	393	340	0.02%	0.002%
16	3.742	745	747	751	rVV2	434	309	0.02%	0.002%
17	3.906	795	798	801	rVB	454	283	0.02%	0.002%
18	3.938	801	808	812	rBV	491	462	0.03%	0.003%
19	3.993	822	825	830	rBV2	351	301	0.02%	0.002%
20	4.163	875	878	883	rVB2	395	288	0.02%	0.002%
21	4.272	909	912	917	rBV2	347	284	0.02%	0.002%
22	4.414	952	956	963	rBV2	461	521	0.03%	0.004%
23	4.462	969	971	975	rVB	428	290	0.02%	0.002%
24	4.485	975	978	982	rBV2	589	451	0.03%	0.003%
25	4.530	988	992	994	rBV	521	396	0.02%	0.003%
26	4.623	1008	1021	1027	rBV	160141	348035	20.54%	2.538%
27	4.941	1116	1120	1123	rBV3	628	381	0.02%	0.003%
28	5.060	1139	1157	1179	rBV	310666	684482	40.40%	4.992%
29	5.231	1208	1210	1213	rVB3	790	387	0.02%	0.003%
30	5.359	1249	1250	1255	rVB2	580	356	0.02%	0.003%
31	5.385	1255	1258	1262	rVB3	776	503	0.03%	0.004%
32	5.446	1275	1277	1281	rBV2	312	271	0.02%	0.002%
33	5.626	1330	1333	1340	rVB3	411	503	0.03%	0.004%
34	5.722	1340	1363	1388	rBV2	629671	1694303	100.00%	12.356%
35	6.079	1470	1474	1478	rBV3	437	341	0.02%	0.002%
36	6.115	1478	1485	1490	rVB4	753	945	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051085.D
 Acq On : 03 Oct 2022 16:19
 Operator : JC/MD
 Sample : N4869-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J00DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.150	1490	1496	1498	rBV2	311	294	0.02%	0.002%
38	6.166	1498	1501	1506	rVB2	438	403	0.02%	0.003%
39	6.247	1512	1526	1552	rBV	466591	883613	52.15%	6.444%
40	6.539	1603	1617	1645	rVB3	84786	171137	10.10%	1.248%
41	6.690	1645	1664	1683	rBV	402560	789223	46.58%	5.756%
42	6.809	1698	1701	1705	rVB4	1913	1537	0.09%	0.011%
43	6.902	1726	1730	1732	rBV2	439	311	0.02%	0.002%
44	6.954	1743	1746	1750	rVB2	454	309	0.02%	0.002%
45	6.980	1750	1754	1756	rVB2	387	289	0.02%	0.002%
46	7.185	1811	1818	1820	rBV5	1285	1341	0.08%	0.010%
47	7.250	1835	1838	1842	rBV2	382	325	0.02%	0.002%
48	7.369	1869	1875	1878	rBV2	430	491	0.03%	0.004%
49	7.497	1906	1915	1922	rBV2	574	867	0.05%	0.006%
50	7.565	1922	1936	1952	rBV	191915	341319	20.15%	2.489%
51	7.796	2005	2008	2016	rVB3	796	802	0.05%	0.006%
52	7.896	2026	2039	2057	rBV	693124	1205685	71.16%	8.793%
53	8.099	2099	2102	2106	rVB2	703	524	0.03%	0.004%
54	8.179	2115	2127	2142	rBV	135115	227884	13.45%	1.662%
55	8.407	2195	2198	2202	rBV2	393	401	0.02%	0.003%
56	8.452	2207	2212	2214	rBV3	439	400	0.02%	0.003%
57	8.552	2229	2243	2257	rBV	992132	1668563	98.48%	12.168%
58	8.636	2258	2269	2304	rVB3	378958	865381	51.08%	6.311%
59	9.015	2381	2387	2389	rBV2	659	666	0.04%	0.005%
60	9.028	2389	2391	2395	rVV2	702	574	0.03%	0.004%
61	9.054	2397	2399	2402	rVB2	528	313	0.02%	0.002%
62	9.070	2402	2404	2407	rVB2	581	326	0.02%	0.002%
63	9.311	2476	2479	2483	rBV2	578	462	0.03%	0.003%
64	9.414	2499	2511	2533	rBV	667658	1102574	65.08%	8.041%
65	9.616	2570	2574	2576	rBV2	584	411	0.02%	0.003%
66	9.648	2581	2584	2587	rBV	457	372	0.02%	0.003%
67	9.668	2587	2590	2594	rVB	684	480	0.03%	0.004%
68	9.751	2612	2616	2618	rBV	347	276	0.02%	0.002%
69	9.806	2629	2633	2635	rBV	371	272	0.02%	0.002%
70	9.915	2663	2667	2668	rBV	556	334	0.02%	0.002%
71	10.092	2719	2722	2724	rBV	610	455	0.03%	0.003%
72	10.221	2759	2762	2771	rVB2	407	602	0.04%	0.004%
73	10.275	2771	2779	2783	rBV	408	644	0.04%	0.005%
74	10.346	2798	2801	2804	rVB	441	294	0.02%	0.002%
75	10.375	2804	2810	2812	rBV	504	567	0.03%	0.004%
76	10.536	2857	2860	2866	rBV3	426	406	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051085.D
 Acq On : 03 Oct 2022 16:19
 Operator : JC/MD
 Sample : N4869-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J00DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.571	2869	2871	2877	rVB2	503	395	0.02%	0.003%
78	10.610	2877	2883	2885	rBV	575	643	0.04%	0.005%
79	10.754	2914	2928	2948	rBV	561959	896050	52.89%	6.535%
80	10.915	2975	2978	2981	rVB3	542	334	0.02%	0.002%
81	10.954	2988	2990	2994	rVB2	582	330	0.02%	0.002%
82	11.063	3020	3024	3025	rBV	446	275	0.02%	0.002%
83	11.108	3035	3038	3042	rVB3	589	368	0.02%	0.003%
84	11.127	3042	3044	3049	rBV2	826	624	0.04%	0.005%
85	11.298	3089	3097	3101	rBV2	534	849	0.05%	0.006%
86	11.343	3107	3111	3116	rVB2	627	589	0.03%	0.004%
87	11.809	3243	3256	3277	rBV	469168	766393	45.23%	5.589%
88	11.947	3296	3299	3303	rBV2	677	432	0.03%	0.003%
89	12.127	3352	3355	3359	rBV2	564	339	0.02%	0.002%
90	12.192	3362	3375	3396	rVV	551692	908247	53.61%	6.624%
91	12.375	3426	3432	3437	rVB4	924	991	0.06%	0.007%
92	12.516	3473	3476	3478	rVB	556	288	0.02%	0.002%
93	12.690	3528	3530	3535	rVB3	900	623	0.04%	0.005%
94	13.069	3645	3648	3651	rBV3	473	399	0.02%	0.003%
95	13.192	3683	3686	3690	rBV2	638	596	0.04%	0.004%
96	13.240	3698	3701	3703	rBV2	615	342	0.02%	0.002%
97	13.336	3728	3731	3736	rBV	591	606	0.04%	0.004%
98	13.671	3832	3835	3837	rBV2	621	448	0.03%	0.003%
99	13.780	3865	3869	3872	rBV2	704	623	0.04%	0.005%
100	14.111	3968	3972	3976	rBV3	583	736	0.04%	0.005%




Sum of corrected areas: 13712236

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051085.D
Acq On : 03 Oct 2022 16:19
Operator : JC/MD
Sample : N4869-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

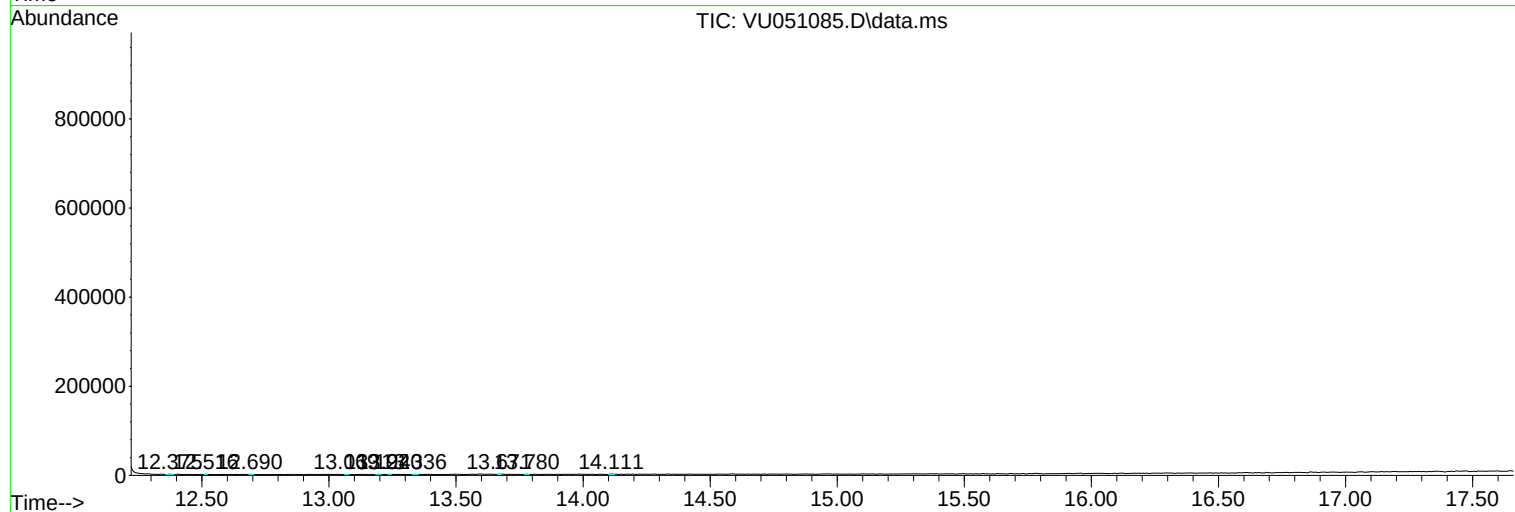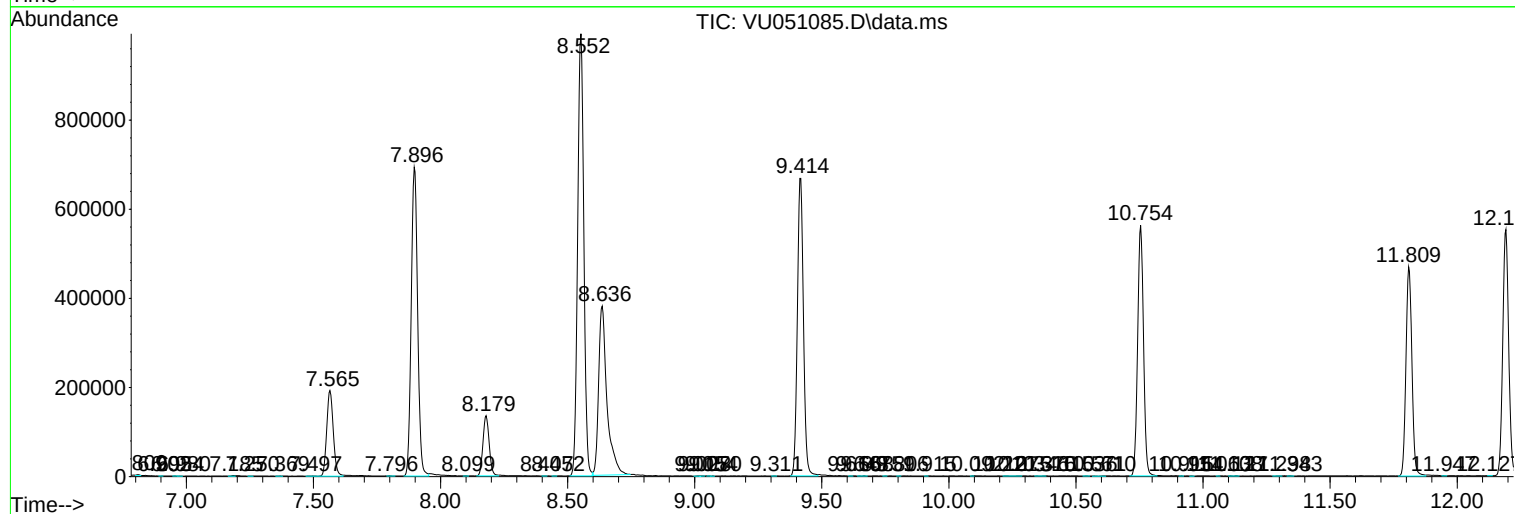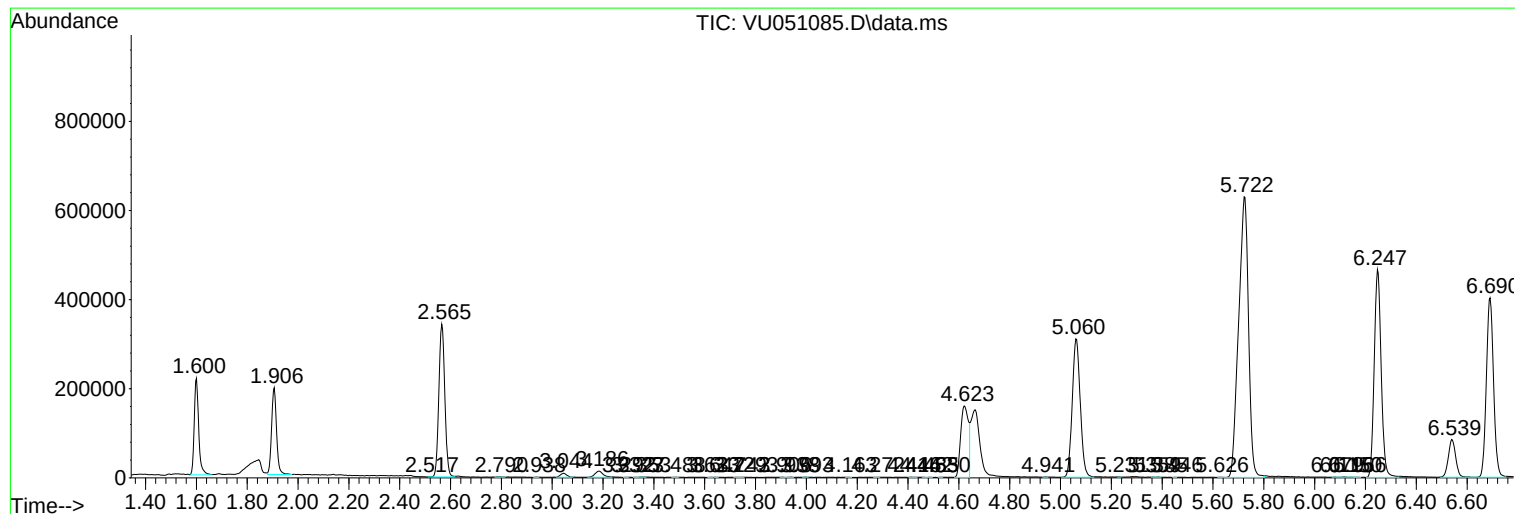

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051085.D
Acq On : 03 Oct 2022 16:19
Operator : JC/MD
Sample : N4869-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051085.D
Acq On : 03 Oct 2022 16:19
Operator : JC/MD
Sample : N4869-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc