

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051086.D
 Acq On : 03 Oct 2022 16:42
 Operator : JC/MD
 Sample : N4869-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	99	rBV	193407	231193	11.53%	1.768%
2	1.903	167	175	191	rVB	173813	230172	11.47%	1.760%
3	2.565	368	381	398	rBV	298173	485133	24.18%	3.710%
4	2.697	420	422	425	rBV	595	289	0.01%	0.002%
5	2.832	457	464	466	rBV3	569	681	0.03%	0.005%
6	2.883	478	480	487	rVB	629	589	0.03%	0.005%
7	2.932	492	495	499	rVB2	404	265	0.01%	0.002%
8	3.028	523	525	526	rBV2	635	319	0.02%	0.002%
9	3.044	526	530	538	rVV4	1655	2134	0.11%	0.016%
10	3.092	542	545	548	rBV	381	296	0.01%	0.002%
11	3.179	563	572	576	rBV	2228	3202	0.16%	0.024%
12	3.285	601	605	609	rBV2	317	361	0.02%	0.003%
13	3.366	619	630	639	rVV5	3191	6909	0.34%	0.053%
14	3.436	649	652	656	rBV2	359	320	0.02%	0.002%
15	3.530	676	681	686	rBV	644	673	0.03%	0.005%
16	3.555	687	689	693	rVB3	475	351	0.02%	0.003%
17	3.581	693	697	702	rBV2	440	467	0.02%	0.004%
18	3.607	702	705	709	rBV2	379	274	0.01%	0.002%
19	3.629	709	712	717	rVB2	366	264	0.01%	0.002%
20	3.803	762	766	770	rBV2	401	396	0.02%	0.003%
21	3.870	785	787	790	rVB	449	254	0.01%	0.002%
22	4.134	864	869	871	rBV2	430	383	0.02%	0.003%
23	4.195	883	888	892	rBV2	339	332	0.02%	0.003%
24	4.234	897	900	903	rBV2	357	273	0.01%	0.002%
25	4.340	926	933	941	rBV2	427	605	0.03%	0.005%
26	4.504	982	984	990	rVB2	365	333	0.02%	0.003%
27	4.536	990	994	997	rBV	267	253	0.01%	0.002%
28	4.620	1007	1020	1049	rBV	143776	369476	18.42%	2.825%
29	4.912	1108	1111	1114	rVB3	555	373	0.02%	0.003%
30	4.935	1114	1118	1121	rBV3	350	320	0.02%	0.002%
31	5.060	1140	1157	1181	rBV	287424	630333	31.42%	4.820%
32	5.378	1248	1256	1260	rBV5	781	1016	0.05%	0.008%
33	5.427	1268	1271	1275	rVB3	365	267	0.01%	0.002%
34	5.449	1276	1278	1286	rVB3	377	343	0.02%	0.003%
35	5.510	1294	1297	1300	rBV3	389	287	0.01%	0.002%
36	5.632	1330	1335	1339	rBV2	372	322	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051086.D
 Acq On : 03 Oct 2022 16:42
 Operator : JC/MD
 Sample : N4869-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	5.722	1342	1363	1395	rBV2	573857	1556976	77.62%	11.906%
38	6.041	1459	1462	1465	rBV2	347	283	0.01%	0.002%
39	6.121	1484	1487	1490	rBV3	452	269	0.01%	0.002%
40	6.246	1512	1526	1548	rBV	413565	784206	39.09%	5.997%
41	6.481	1595	1599	1601	rVB2	521	322	0.02%	0.002%
42	6.529	1604	1614	1627	rVB6	12798	27069	1.35%	0.207%
43	6.603	1635	1637	1640	rVB2	491	278	0.01%	0.002%
44	6.626	1640	1644	1649	rBV2	338	301	0.02%	0.002%
45	6.690	1649	1664	1684	rBV	372178	723084	36.05%	5.529%
46	6.857	1714	1716	1720	rVB2	530	295	0.01%	0.002%
47	6.886	1722	1725	1728	rVB3	550	315	0.02%	0.002%
48	6.922	1734	1736	1739	rBV	540	306	0.02%	0.002%
49	6.996	1756	1759	1765	rBV3	409	391	0.02%	0.003%
50	7.037	1769	1772	1777	rBV2	545	588	0.03%	0.004%
51	7.452	1898	1901	1908	rBV2	441	448	0.02%	0.003%
52	7.497	1913	1915	1920	rVB2	419	277	0.01%	0.002%
53	7.565	1924	1936	1955	rBV	178537	316631	15.78%	2.421%
54	7.664	1964	1967	1968	rBV3	467	320	0.02%	0.002%
55	7.690	1972	1975	1978	rBV3	1180	727	0.04%	0.006%
56	7.896	2025	2039	2072	rBV	636705	1101575	54.92%	8.423%
57	8.179	2115	2127	2143	rVV	125742	213784	10.66%	1.635%
58	8.378	2186	2189	2193	rVB3	549	472	0.02%	0.004%
59	8.410	2196	2199	2201	rVB	451	256	0.01%	0.002%
60	8.423	2201	2203	2207	rVB	423	281	0.01%	0.002%
61	8.475	2207	2219	2226	rBV5	2356	3319	0.17%	0.025%
62	8.552	2226	2243	2257	rBV	1190166	2005937	100.00%	15.339%
63	8.632	2258	2268	2305	rVB4	369649	848236	42.29%	6.486%
64	8.931	2358	2361	2362	rBV	577	256	0.01%	0.002%
65	9.024	2387	2390	2393	rBV	398	289	0.01%	0.002%
66	9.095	2408	2412	2417	rVB2	779	548	0.03%	0.004%
67	9.127	2419	2422	2424	rVB2	471	253	0.01%	0.002%
68	9.147	2424	2428	2429	rBV	334	253	0.01%	0.002%
69	9.221	2448	2451	2454	rVB3	496	338	0.02%	0.003%
70	9.259	2460	2463	2469	rVB3	628	581	0.03%	0.004%
71	9.288	2469	2472	2474	rBV2	599	423	0.02%	0.003%
72	9.417	2498	2512	2539	rBV	629034	1037005	51.70%	7.930%
73	9.558	2553	2556	2558	rBV2	523	367	0.02%	0.003%
74	9.619	2572	2575	2578	rVB3	603	417	0.02%	0.003%
75	9.639	2578	2581	2585	rBV2	411	335	0.02%	0.003%
76	9.774	2619	2623	2626	rBV	465	317	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051086.D
 Acq On : 03 Oct 2022 16:42
 Operator : JC/MD
 Sample : N4869-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.124	2729	2732	2734	rBV2	380	303	0.02%	0.002%
78	10.198	2752	2755	2759	rBV2	468	330	0.02%	0.003%
79	10.426	2821	2826	2829	rBV3	525	463	0.02%	0.004%
80	10.494	2842	2847	2852	rBV3	707	618	0.03%	0.005%
81	10.549	2860	2864	2870	rVB2	491	406	0.02%	0.003%
82	10.584	2870	2875	2877	rBV2	536	447	0.02%	0.003%
83	10.754	2913	2928	2946	rBV	533137	868930	43.32%	6.645%
84	10.893	2964	2971	2984	rVB6	2025	3219	0.16%	0.025%
85	10.963	2989	2993	2995	rBV3	346	275	0.01%	0.002%
86	11.102	3034	3036	3039	rBV2	424	305	0.02%	0.002%
87	11.230	3072	3076	3080	rBV2	492	438	0.02%	0.003%
88	11.394	3122	3127	3129	rBV	474	416	0.02%	0.003%
89	11.455	3141	3146	3149	rBV3	753	584	0.03%	0.004%
90	11.568	3178	3181	3184	rBV	795	640	0.03%	0.005%
91	11.809	3244	3256	3274	rBV	451852	721722	35.98%	5.519%
92	12.192	3362	3375	3395	rBV	534321	876914	43.72%	6.706%
93	12.497	3465	3470	3475	rBV4	652	940	0.05%	0.007%
94	12.957	3611	3613	3616	rBV	456	260	0.01%	0.002%
95	13.304	3716	3721	3722	rBV2	420	383	0.02%	0.003%
96	13.349	3731	3735	3739	rBV3	551	592	0.03%	0.005%
97	13.384	3743	3746	3749	rVV4	539	348	0.02%	0.003%
98	13.478	3773	3775	3778	rVB2	542	246	0.01%	0.002%
99	13.905	3906	3908	3912	rBV3	506	378	0.02%	0.003%
100	15.265	4329	4331	4334	rBV2	858	471	0.02%	0.004%




Sum of corrected areas: 13077414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051086.D
Acq On : 03 Oct 2022 16:42
Operator : JC/MD
Sample : N4869-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

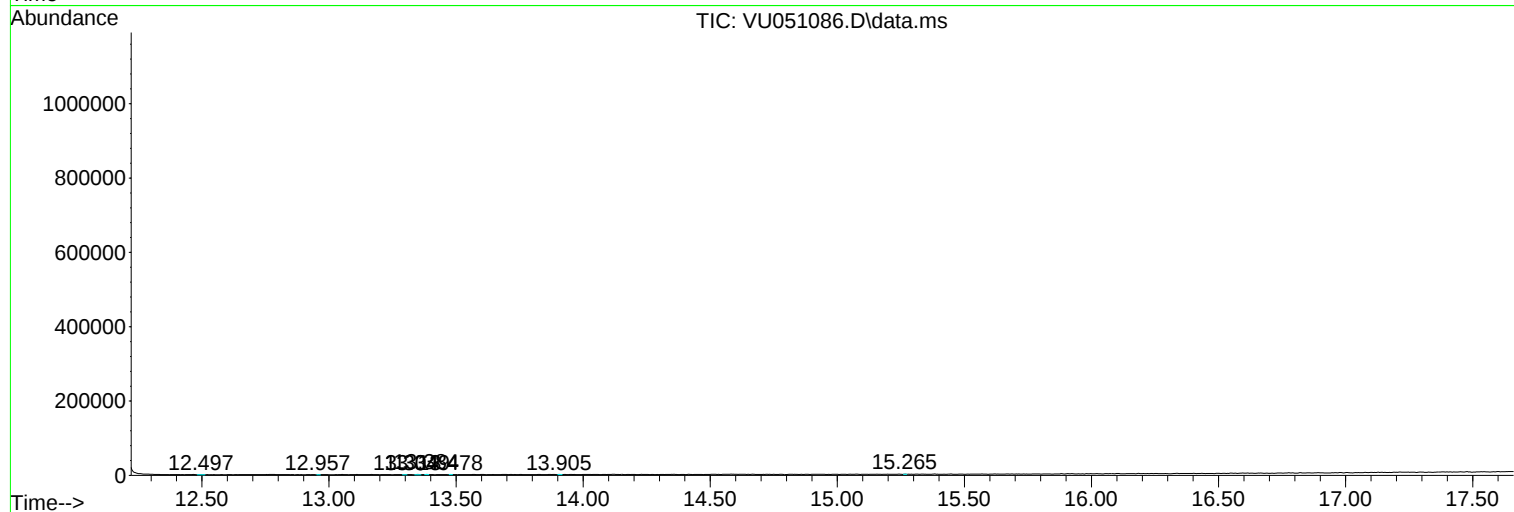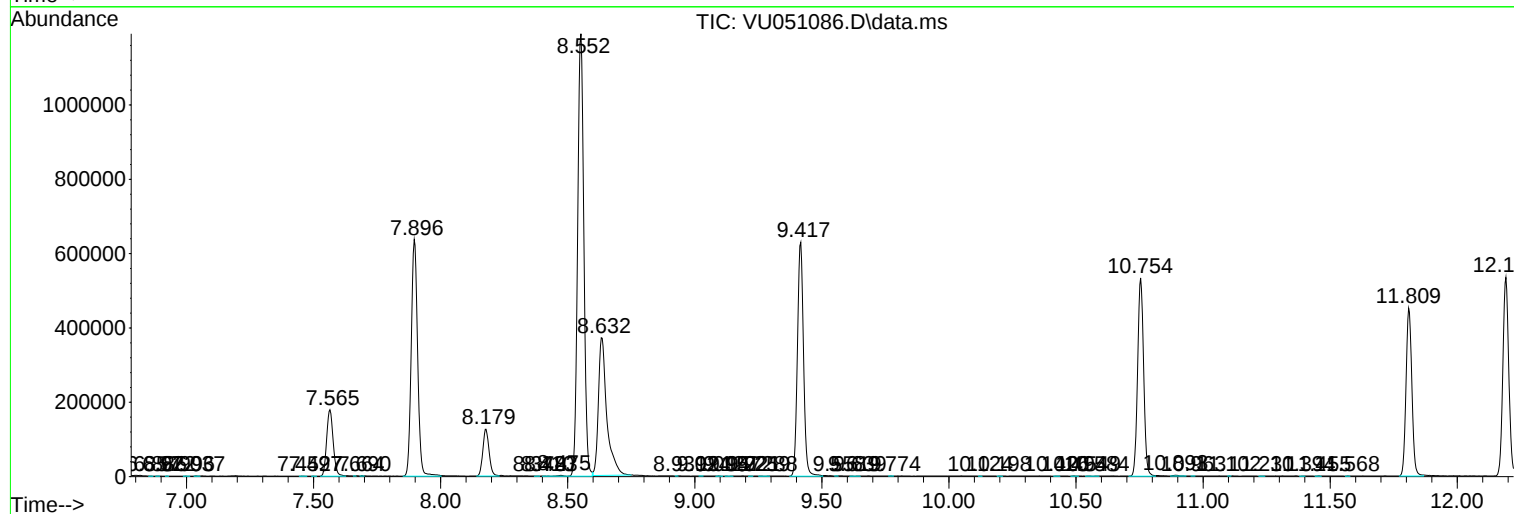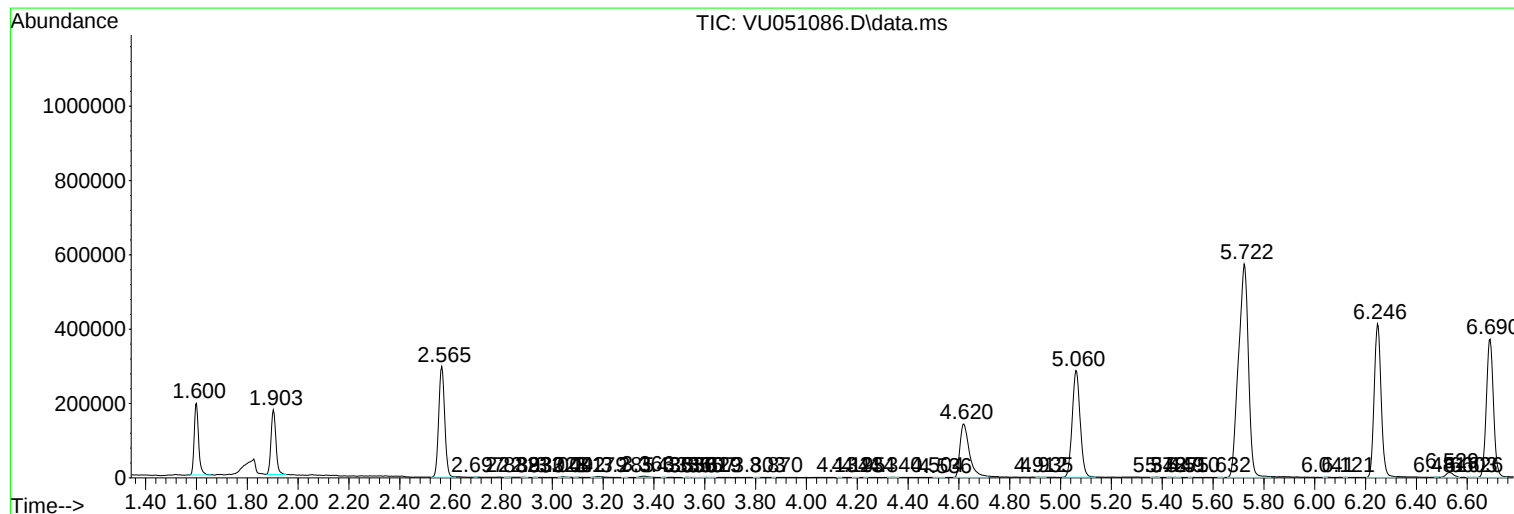

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051086.D
Acq On : 03 Oct 2022 16:42
Operator : JC/MD
Sample : N4869-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051086.D
Acq On : 03 Oct 2022 16:42
Operator : JC/MD
Sample : N4869-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc