

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051089.D
 Acq On : 03 Oct 2022 17:52
 Operator : JC/MD
 Sample : N4859-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rBV	217486	257376	15.59%	2.135%
2	1.903	166	175	197	rVB	183128	253064	15.33%	2.099%
3	2.565	367	381	399	rBV	330773	536618	32.51%	4.451%
4	2.745	435	437	442	rVB2	504	339	0.02%	0.003%
5	2.771	442	445	446	rBV3	764	421	0.03%	0.003%
6	2.935	491	496	498	rBV2	369	362	0.02%	0.003%
7	3.041	521	529	540	rVB3	5531	9876	0.60%	0.082%
8	3.182	561	573	588	rVB2	6759	14152	0.86%	0.117%
9	3.340	617	622	625	rBV3	272	265	0.02%	0.002%
10	3.404	640	642	645	rVB	559	297	0.02%	0.002%
11	3.440	648	653	655	rVB	353	273	0.02%	0.002%
12	3.523	676	679	681	rBV	621	420	0.03%	0.003%
13	3.581	694	697	701	rBV	512	421	0.03%	0.003%
14	3.610	702	706	712	rVB2	385	443	0.03%	0.004%
15	3.694	728	732	736	rVV	376	266	0.02%	0.002%
16	3.838	773	777	780	rBV2	290	277	0.02%	0.002%
17	4.034	832	838	840	rBV2	351	388	0.02%	0.003%
18	4.378	942	945	948	rBV	426	338	0.02%	0.003%
19	4.417	955	957	963	rVB2	378	349	0.02%	0.003%
20	4.513	985	987	994	rVB	428	316	0.02%	0.003%
21	4.616	1004	1019	1053	rBV	166906	424965	25.74%	3.525%
22	4.845	1087	1090	1093	rBV2	742	396	0.02%	0.003%
23	4.931	1114	1117	1119	rBV2	417	296	0.02%	0.002%
24	4.964	1125	1127	1131	rVB2	466	272	0.02%	0.002%
25	5.060	1139	1157	1179	rBV2	301741	662961	40.16%	5.499%
26	5.169	1188	1191	1194	rBV	1129	734	0.04%	0.006%
27	5.330	1238	1241	1247	rVB4	537	448	0.03%	0.004%
28	5.465	1281	1283	1290	rVB2	280	252	0.02%	0.002%
29	5.549	1304	1309	1312	rBV2	475	395	0.02%	0.003%
30	5.568	1312	1315	1324	rVB2	481	560	0.03%	0.005%
31	5.722	1339	1363	1395	rBV2	600262	1650689	100.00%	13.693%
32	5.941	1429	1431	1437	rBV2	542	496	0.03%	0.004%
33	6.038	1456	1461	1469	rVB4	633	968	0.06%	0.008%
34	6.147	1491	1495	1502	rVB3	465	547	0.03%	0.005%
35	6.179	1502	1505	1510	rBV4	476	333	0.02%	0.003%
36	6.247	1512	1526	1557	rBV	459757	877775	53.18%	7.281%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051089.D
 Acq On : 03 Oct 2022 17:52
 Operator : JC/MD
 Sample : N4859-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.375	1563	1566	1569	rVV2	1055	658	0.04%	0.005%
38	6.398	1569	1573	1578	rVB5	798	852	0.05%	0.007%
39	6.439	1584	1586	1588	rBV2	514	284	0.02%	0.002%
40	6.526	1602	1613	1631	rVB2	14757	28506	1.73%	0.236%
41	6.591	1631	1633	1636	rBV2	600	344	0.02%	0.003%
42	6.610	1636	1639	1644	rVB4	671	617	0.04%	0.005%
43	6.687	1649	1663	1688	rBV	391815	770852	46.70%	6.394%
44	6.867	1717	1719	1723	rVB3	426	285	0.02%	0.002%
45	6.951	1739	1745	1749	rBV3	485	504	0.03%	0.004%
46	7.047	1772	1775	1782	rVB2	653	704	0.04%	0.006%
47	7.086	1782	1787	1789	rBV2	424	422	0.03%	0.004%
48	7.137	1797	1803	1805	rBV	326	333	0.02%	0.003%
49	7.182	1812	1817	1819	rBV3	1153	942	0.06%	0.008%
50	7.230	1829	1832	1837	rVB2	281	280	0.02%	0.002%
51	7.279	1841	1847	1850	rBV2	432	418	0.03%	0.003%
52	7.388	1878	1881	1884	rBV2	372	275	0.02%	0.002%
53	7.517	1917	1921	1923	rBV	330	272	0.02%	0.002%
54	7.565	1923	1936	1954	rBV	187653	330860	20.04%	2.745%
55	7.896	2025	2039	2060	rBV	676658	1172863	71.05%	9.729%
56	8.105	2102	2104	2108	rBV3	375	281	0.02%	0.002%
57	8.179	2114	2127	2149	rBV	133833	226748	13.74%	1.881%
58	8.336	2172	2176	2179	rBV2	510	521	0.03%	0.004%
59	8.427	2201	2204	2207	rVB3	668	469	0.03%	0.004%
60	8.443	2207	2209	2214	rBV2	475	402	0.02%	0.003%
61	8.472	2214	2218	2220	rBV2	540	446	0.03%	0.004%
62	8.497	2223	2226	2231	rBV2	429	485	0.03%	0.004%
63	8.549	2236	2242	2250	rBV5	2629	3670	0.22%	0.030%
64	8.632	2254	2268	2309	rBV3	396260	907438	54.97%	7.527%
65	8.848	2332	2335	2336	rBV2	395	268	0.02%	0.002%
66	9.237	2452	2456	2459	rBV2	370	287	0.02%	0.002%
67	9.417	2499	2512	2535	rBV	683834	1131239	68.53%	9.384%
68	9.603	2566	2570	2571	rBV2	461	355	0.02%	0.003%
69	9.668	2587	2590	2593	rBV	320	255	0.02%	0.002%
70	9.700	2596	2600	2603	rVV2	423	324	0.02%	0.003%
71	9.796	2627	2630	2633	rBV	401	261	0.02%	0.002%
72	9.992	2688	2691	2694	rBV	345	258	0.02%	0.002%
73	10.037	2699	2705	2708	rBV2	391	437	0.03%	0.004%
74	10.086	2717	2720	2722	rVB2	498	288	0.02%	0.002%
75	10.115	2727	2729	2733	rBV2	321	286	0.02%	0.002%
76	10.147	2736	2739	2742	rBV2	330	259	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051089.D
 Acq On : 03 Oct 2022 17:52
 Operator : JC/MD
 Sample : N4859-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.462	2833	2837	2839	rBV2	350	274	0.02%	0.002%
78	10.574	2866	2872	2873	rBV	341	322	0.02%	0.003%
79	10.754	2913	2928	2950	rBV	566975	919658	55.71%	7.629%
80	10.944	2984	2987	2991	rBV3	486	432	0.03%	0.004%
81	11.047	3016	3019	3021	rBV	577	430	0.03%	0.004%
82	11.182	3055	3061	3064	rBV2	465	431	0.03%	0.004%
83	11.323	3102	3105	3108	rVB2	437	253	0.02%	0.002%
84	11.343	3108	3111	3112	rBV	400	265	0.02%	0.002%
85	11.809	3243	3256	3277	rBV	536839	858581	52.01%	7.122%
86	11.947	3297	3299	3302	rVB3	782	399	0.02%	0.003%
87	12.021	3319	3322	3326	rBV2	458	330	0.02%	0.003%
88	12.060	3331	3334	3336	rBV	585	406	0.02%	0.003%
89	12.192	3361	3375	3396	rBV	596518	984166	59.62%	8.164%
90	12.648	3514	3517	3520	rBV3	573	374	0.02%	0.003%
91	12.786	3556	3560	3563	rBV2	631	438	0.03%	0.004%
92	12.831	3571	3574	3576	rBV	565	435	0.03%	0.004%
93	12.864	3581	3584	3587	rVB2	537	351	0.02%	0.003%
94	13.140	3668	3670	3676	rVB3	523	435	0.03%	0.004%
95	13.237	3697	3700	3704	rBV2	827	586	0.04%	0.005%
96	13.362	3736	3739	3745	rBV2	596	618	0.04%	0.005%
97	13.410	3750	3754	3759	rBV4	834	835	0.05%	0.007%
98	13.680	3836	3838	3841	rVB2	679	357	0.02%	0.003%
99	13.700	3841	3844	3845	rBV	484	319	0.02%	0.003%
100	15.484	4397	4399	4402	rBV3	1171	839	0.05%	0.007%




Sum of corrected areas: 12055130

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051089.D
Acq On : 03 Oct 2022 17:52
Operator : JC/MD
Sample : N4859-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

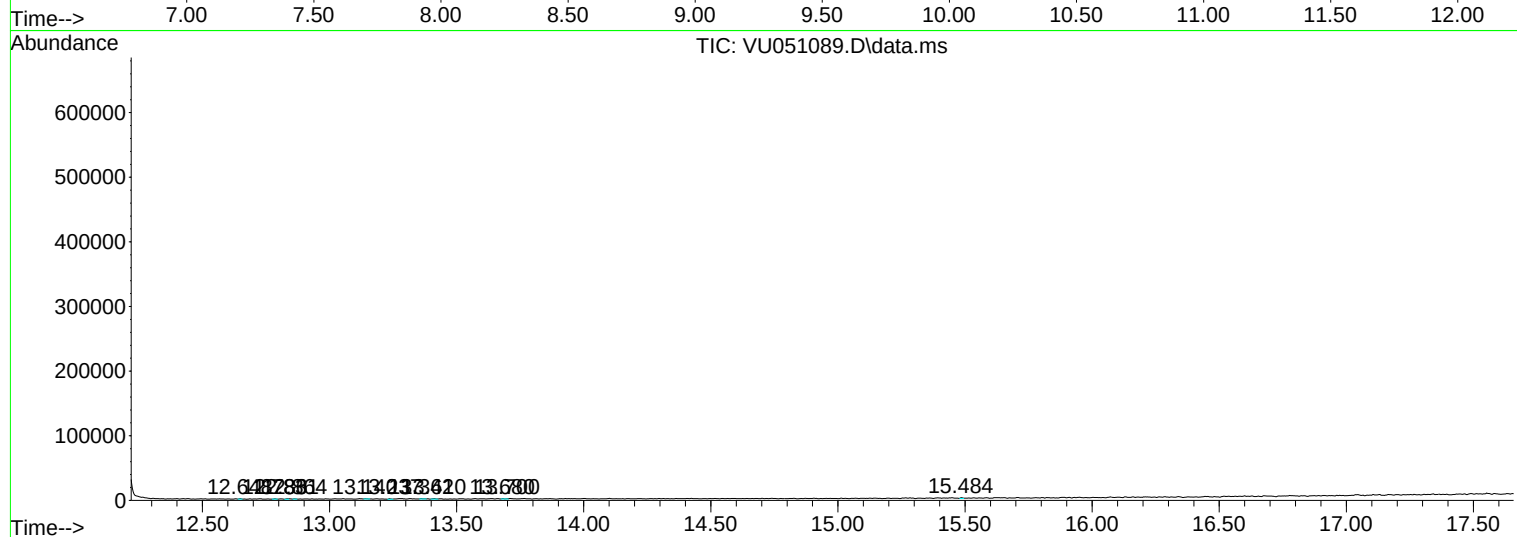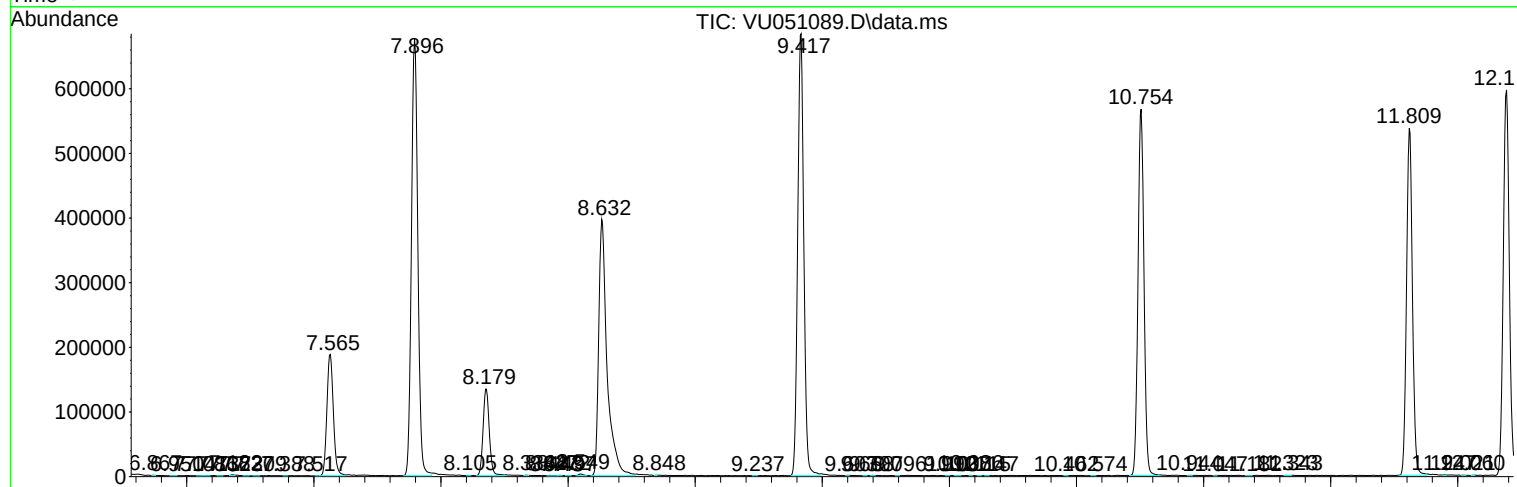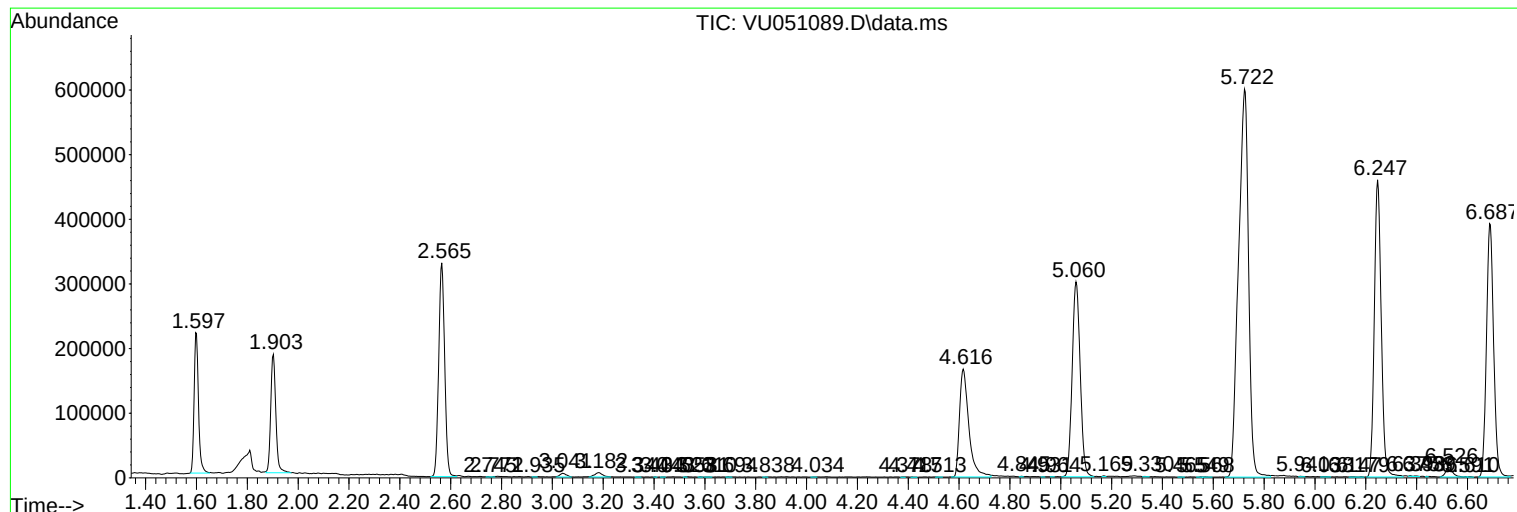

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051089.D
Acq On : 03 Oct 2022 17:52
Operator : JC/MD
Sample : N4859-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051089.D
Acq On : 03 Oct 2022 17:52
Operator : JC/MD
Sample : N4859-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc