

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051092.D
 Acq On : 03 Oct 2022 19:02
 Operator : JC/MD
 Sample : N4854-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051092.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	206083	259097	16.32%	2.041%
2	1.903	167	175	198	rVB	177141	240949	15.17%	1.898%
3	2.565	368	381	397	rBV	307957	496335	31.26%	3.910%
4	2.794	448	452	459	rVB4	898	1163	0.07%	0.009%
5	2.896	482	484	490	rVB3	459	351	0.02%	0.003%
6	2.925	490	493	498	rBV2	583	661	0.04%	0.005%
7	3.041	520	529	537	rBV4	1994	3554	0.22%	0.028%
8	3.173	563	570	572	rBV2	1587	1756	0.11%	0.014%
9	3.353	617	626	627	rBV4	6818	7504	0.47%	0.059%
10	3.539	681	684	692	rBV2	387	492	0.03%	0.004%
11	3.584	696	698	702	rVB3	587	418	0.03%	0.003%
12	3.613	702	707	710	rVB2	567	490	0.03%	0.004%
13	3.697	728	733	737	rVV3	565	619	0.04%	0.005%
14	3.867	782	786	794	rVB3	700	931	0.06%	0.007%
15	3.929	799	805	807	rBV2	257	325	0.02%	0.003%
16	4.166	874	879	881	rBV2	467	512	0.03%	0.004%
17	4.279	910	914	919	rBV	492	465	0.03%	0.004%
18	4.330	928	930	934	rVB2	652	416	0.03%	0.003%
19	4.356	934	938	943	rBV2	402	394	0.02%	0.003%
20	4.385	943	947	951	rBV	278	302	0.02%	0.002%
21	4.617	1007	1019	1061	rVV	151060	389685	24.54%	3.070%
22	5.060	1139	1157	1179	rBV	292168	641587	40.40%	5.054%
23	5.234	1208	1211	1213	rBV3	585	367	0.02%	0.003%
24	5.372	1251	1254	1257	rVB2	637	330	0.02%	0.003%
25	5.440	1268	1275	1279	rBV2	558	643	0.04%	0.005%
26	5.523	1298	1301	1305	rVB2	463	356	0.02%	0.003%
27	5.588	1315	1321	1323	rBV2	402	332	0.02%	0.003%
28	5.613	1323	1329	1333	rVB2	284	326	0.02%	0.003%
29	5.723	1341	1363	1387	rBV2	585774	1587926	100.00%	12.509%
30	5.983	1442	1444	1447	rVB2	888	506	0.03%	0.004%
31	6.108	1480	1483	1489	rVV3	528	631	0.04%	0.005%
32	6.247	1512	1526	1547	rBV	431167	823578	51.87%	6.488%
33	6.459	1588	1592	1595	rVB3	817	659	0.04%	0.005%
34	6.478	1595	1598	1601	rBV2	544	354	0.02%	0.003%
35	6.539	1603	1617	1636	rVV3	49722	102297	6.44%	0.806%
36	6.687	1648	1663	1681	rBV	379206	743467	46.82%	5.857%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051092.D
 Acq On : 03 Oct 2022 19:02
 Operator : JC/MD
 Sample : N4854-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.899	1727	1729	1732	rVB	672	361	0.02%	0.003%
38	6.925	1732	1737	1739	rBV2	487	404	0.03%	0.003%
39	6.944	1739	1743	1746	rVB3	473	373	0.02%	0.003%
40	7.073	1778	1783	1787	rBV2	317	379	0.02%	0.003%
41	7.189	1808	1819	1826	rVB5	1626	3229	0.20%	0.025%
42	7.237	1831	1834	1836	rBV	489	298	0.02%	0.002%
43	7.305	1853	1855	1863	rVB2	779	756	0.05%	0.006%
44	7.353	1863	1870	1874	rVB	514	505	0.03%	0.004%
45	7.379	1874	1878	1884	rBV	281	313	0.02%	0.002%
46	7.565	1921	1936	1961	rVV	180972	320565	20.19%	2.525%
47	7.793	2002	2007	2009	rBV2	846	756	0.05%	0.006%
48	7.896	2023	2039	2057	rBV	644357	1117950	70.40%	8.806%
49	8.079	2094	2096	2101	rVB4	900	503	0.03%	0.004%
50	8.108	2103	2105	2111	rBV3	279	294	0.02%	0.002%
51	8.176	2115	2126	2151	rBV2	130538	224590	14.14%	1.769%
52	8.395	2190	2194	2195	rBV2	619	444	0.03%	0.003%
53	8.424	2200	2203	2208	rVB4	715	641	0.04%	0.005%
54	8.462	2208	2215	2217	rBV4	975	1209	0.08%	0.010%
55	8.552	2229	2243	2256	rBV	724378	1219930	76.83%	9.610%
56	8.633	2257	2268	2298	rVB2	386283	828146	52.15%	6.524%
57	8.841	2330	2333	2338	rBV5	888	636	0.04%	0.005%
58	8.922	2355	2358	2359	rBV2	641	335	0.02%	0.003%
59	9.047	2395	2397	2403	rVB3	529	462	0.03%	0.004%
60	9.179	2436	2438	2444	rVB4	475	410	0.03%	0.003%
61	9.414	2498	2511	2537	rBV	645103	1068555	67.29%	8.417%
62	9.694	2596	2598	2606	rVB2	745	835	0.05%	0.007%
63	9.742	2611	2613	2619	rVB3	463	362	0.02%	0.003%
64	9.774	2619	2623	2628	rVB3	969	891	0.06%	0.007%
65	9.803	2628	2632	2634	rBV	381	360	0.02%	0.003%
66	9.841	2640	2644	2648	rBV2	561	633	0.04%	0.005%
67	9.980	2684	2687	2689	rBV2	559	389	0.02%	0.003%
68	10.099	2721	2724	2726	rBV3	687	511	0.03%	0.004%
69	10.205	2750	2757	2762	rBV3	497	597	0.04%	0.005%
70	10.263	2771	2775	2777	rBV2	397	317	0.02%	0.002%
71	10.385	2807	2813	2814	rBV	468	417	0.03%	0.003%
72	10.488	2838	2845	2851	rVB3	803	843	0.05%	0.007%
73	10.755	2914	2928	2946	rBV	542003	886606	55.83%	6.984%
74	10.890	2963	2970	2974	rBV4	1277	1623	0.10%	0.013%
75	11.401	3126	3129	3131	rBV	434	301	0.02%	0.002%
76	11.468	3146	3150	3155	rBV4	772	689	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051092.D
 Acq On : 03 Oct 2022 19:02
 Operator : JC/MD
 Sample : N4854-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.510	3159	3163	3170	rBV	703	653	0.04%	0.005%
78	11.546	3170	3174	3177	rBV3	458	396	0.02%	0.003%
79	11.668	3207	3212	3215	rBV2	582	507	0.03%	0.004%
80	11.748	3233	3237	3242	rVB4	828	803	0.05%	0.006%
81	11.809	3244	3256	3277	rBV	487297	771310	48.57%	6.076%
82	12.192	3361	3375	3401	rBV	551980	913654	57.54%	7.197%
83	12.372	3428	3431	3433	rBV	749	422	0.03%	0.003%
84	12.401	3437	3440	3444	rVB	555	399	0.03%	0.003%
85	12.446	3450	3454	3455	rBV2	567	405	0.03%	0.003%
86	12.504	3469	3472	3477	rVB3	663	542	0.03%	0.004%
87	12.828	3570	3573	3577	rBV4	517	566	0.04%	0.004%
88	13.041	3635	3639	3645	rBV	953	992	0.06%	0.008%
89	13.105	3657	3659	3664	rVB3	662	582	0.04%	0.005%
90	13.137	3664	3669	3671	rBV2	688	730	0.05%	0.006%
91	13.234	3693	3699	3701	rBV2	660	611	0.04%	0.005%
92	13.285	3712	3715	3718	rVB	795	507	0.03%	0.004%
93	13.912	3908	3910	3913	rBV2	587	400	0.03%	0.003%
94	13.986	3930	3933	3937	rBV2	457	399	0.03%	0.003%
95	14.131	3976	3978	3981	rBV	409	345	0.02%	0.003%
96	14.201	3997	4000	4005	rVB2	736	527	0.03%	0.004%
97	14.832	4191	4196	4197	rBV2	616	588	0.04%	0.005%
98	15.121	4283	4286	4289	rBV3	899	802	0.05%	0.006%
99	15.185	4303	4306	4308	rBV2	942	598	0.04%	0.005%
100	15.774	4486	4489	4491	rBV2	1257	739	0.05%	0.006%




Sum of corrected areas: 12694673

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051092.D
Acq On : 03 Oct 2022 19:02
Operator : JC/MD
Sample : N4854-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

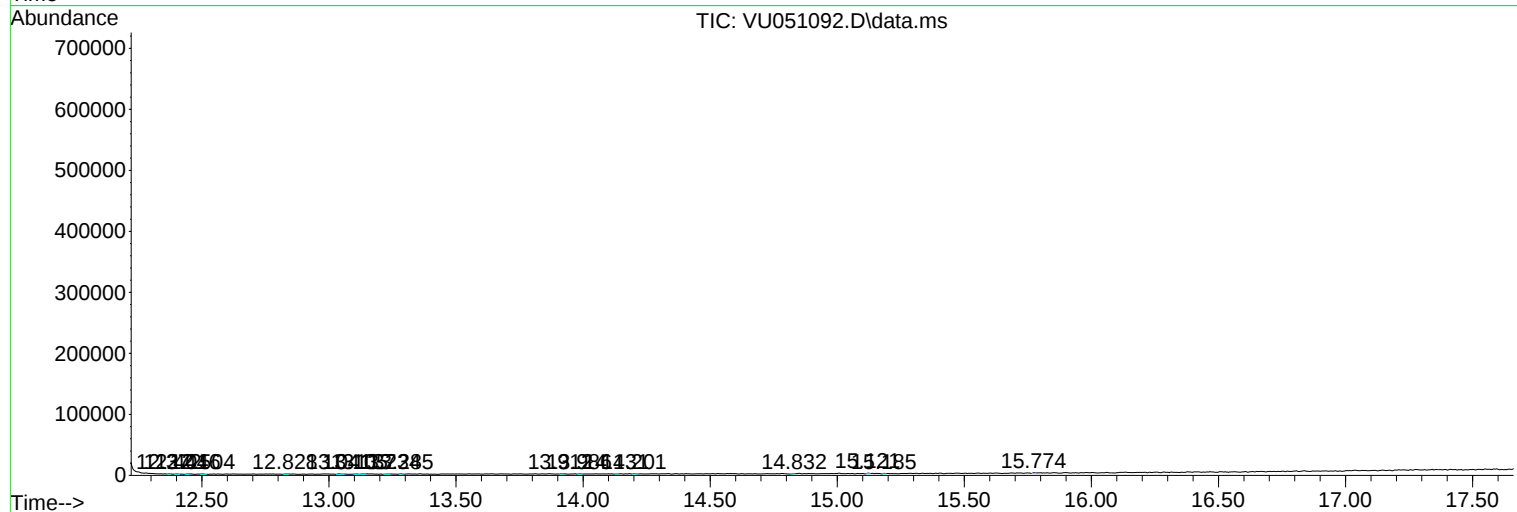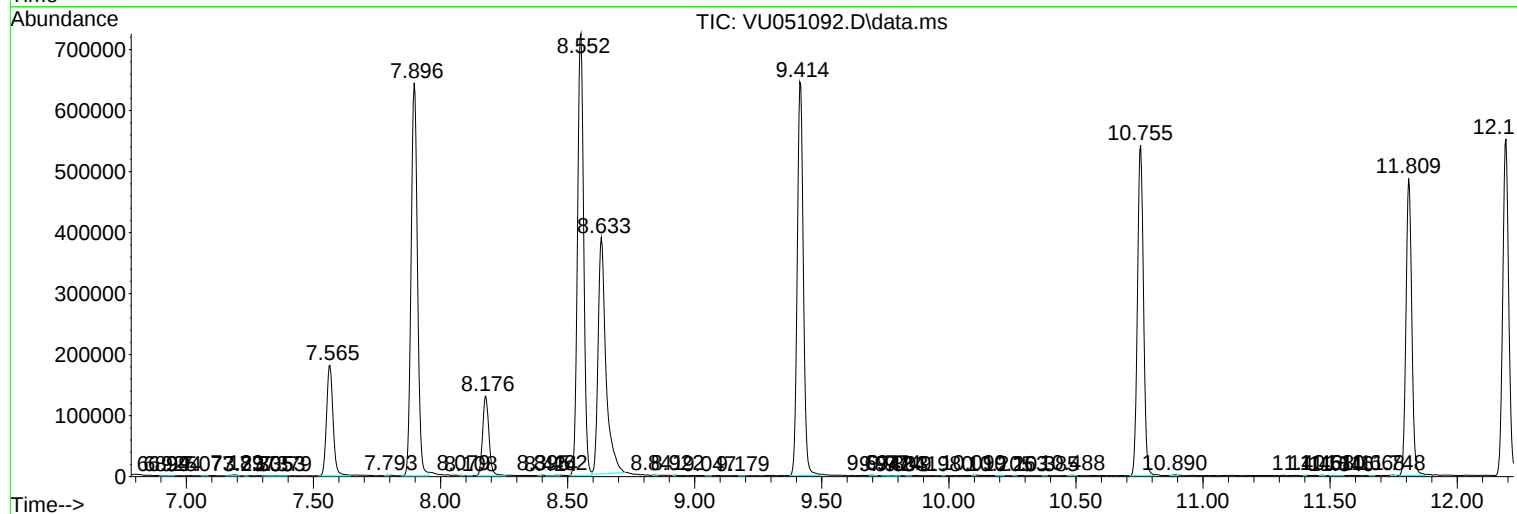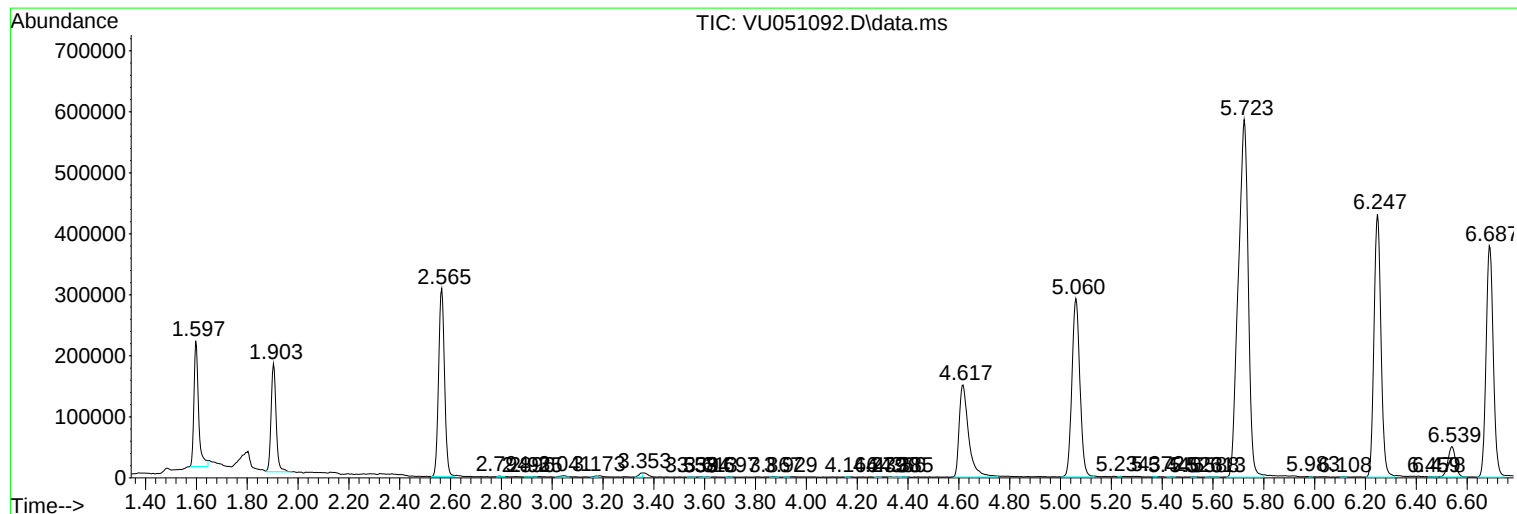

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051092.D
Acq On : 03 Oct 2022 19:02
Operator : JC/MD
Sample : N4854-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051092.D
Acq On : 03 Oct 2022 19:02
Operator : JC/MD
Sample : N4854-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc