

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051094.D
 Acq On : 03 Oct 2022 19:48
 Operator : JC/MD
 Sample : N4854-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rBV	197274	257250	16.98%	2.287%
2	1.903	167	175	190	rBV	164326	219854	14.51%	1.954%
3	2.565	368	381	397	rBV	295642	476453	31.45%	4.236%
4	2.784	443	449	453	rBV4	1132	1288	0.09%	0.011%
5	2.880	473	479	484	rBV5	629	908	0.06%	0.008%
6	2.906	484	487	491	rVV	735	617	0.04%	0.005%
7	2.951	498	501	506	rVV3	631	714	0.05%	0.006%
8	2.977	506	509	513	rVV3	491	509	0.03%	0.005%
9	2.999	513	516	518	rVV2	525	365	0.02%	0.003%
10	3.044	519	530	538	rVB9	2203	4691	0.31%	0.042%
11	3.182	562	573	582	rBV	4445	9612	0.63%	0.085%
12	3.273	595	601	604	rBV2	506	587	0.04%	0.005%
13	3.298	607	609	612	rVV2	721	488	0.03%	0.004%
14	3.314	612	614	619	rVB3	595	362	0.02%	0.003%
15	3.359	621	628	634	rBV5	1516	2243	0.15%	0.020%
16	3.488	662	668	673	rBV2	737	786	0.05%	0.007%
17	3.517	673	677	680	rVB2	528	427	0.03%	0.004%
18	3.584	692	698	701	rBV2	668	596	0.04%	0.005%
19	3.607	701	705	708	rVV3	390	386	0.03%	0.003%
20	3.803	763	766	768	rBV	593	439	0.03%	0.004%
21	4.009	825	830	833	rVB	408	361	0.02%	0.003%
22	4.179	876	883	890	rVB2	372	661	0.04%	0.006%
23	4.546	991	997	1003	rVB2	375	508	0.03%	0.005%
24	4.616	1007	1019	1048	rBV	145444	368897	24.35%	3.279%
25	4.867	1094	1097	1099	rBV2	618	394	0.03%	0.004%
26	4.986	1131	1134	1139	rBV2	391	384	0.03%	0.003%
27	5.060	1139	1157	1178	rBV	275719	610966	40.32%	5.431%
28	5.285	1221	1227	1238	rVB6	1448	3260	0.22%	0.029%
29	5.340	1239	1244	1246	rBV3	642	440	0.03%	0.004%
30	5.372	1251	1254	1256	rBV2	639	506	0.03%	0.004%
31	5.385	1256	1258	1265	rVB4	906	573	0.04%	0.005%
32	5.424	1265	1270	1273	rBV2	478	469	0.03%	0.004%
33	5.459	1273	1281	1289	rVB6	2218	3809	0.25%	0.034%
34	5.723	1341	1363	1385	rBV2	553479	1515152	100.00%	13.469%
35	5.883	1410	1413	1415	rBV4	1570	1241	0.08%	0.011%
36	5.941	1429	1431	1435	rBV3	549	396	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051094.D
 Acq On : 03 Oct 2022 19:48
 Operator : JC/MD
 Sample : N4854-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	5.967	1436	1439	1442	rVB3	639	410	0.03%	0.004%
38	6.038	1457	1461	1467	rVB3	645	776	0.05%	0.007%
39	6.166	1498	1501	1508	rBV3	389	523	0.03%	0.005%
40	6.247	1511	1526	1550	rBV	414595	779905	51.47%	6.933%
41	6.343	1553	1556	1560	rBV5	1073	710	0.05%	0.006%
42	6.539	1605	1617	1631	rVB6	24977	52845	3.49%	0.470%
43	6.600	1631	1636	1640	rBV4	586	575	0.04%	0.005%
44	6.687	1649	1663	1685	rBV	365092	713318	47.08%	6.341%
45	6.928	1733	1738	1744	rVB3	610	739	0.05%	0.007%
46	7.182	1809	1817	1820	rBV4	1178	1696	0.11%	0.015%
47	7.253	1831	1839	1851	rVB6	1827	3531	0.23%	0.031%
48	7.382	1869	1879	1888	rVB5	1790	3250	0.21%	0.029%
49	7.423	1888	1892	1896	rBV2	405	405	0.03%	0.004%
50	7.478	1905	1909	1915	rBV2	481	384	0.03%	0.003%
51	7.565	1923	1936	1959	rBV	167546	301400	19.89%	2.679%
52	7.816	2011	2014	2019	rVB2	546	423	0.03%	0.004%
53	7.896	2025	2039	2071	rBV	610120	1061453	70.06%	9.436%
54	8.179	2116	2127	2144	rBV	121334	207855	13.72%	1.848%
55	8.462	2211	2215	2220	rBV3	1277	1153	0.08%	0.010%
56	8.552	2231	2243	2257	rBV	226330	379626	25.06%	3.375%
57	8.632	2257	2268	2302	rVV2	353686	784441	51.77%	6.974%
58	9.050	2393	2398	2402	rBV2	421	406	0.03%	0.004%
59	9.166	2429	2434	2438	rVB2	656	480	0.03%	0.004%
60	9.275	2463	2468	2472	rBV2	575	563	0.04%	0.005%
61	9.414	2498	2511	2531	rBV	605318	1005096	66.34%	8.935%
62	9.552	2551	2554	2561	rVB5	866	803	0.05%	0.007%
63	9.681	2590	2594	2596	rBV	736	519	0.03%	0.005%
64	9.767	2618	2621	2626	rVV2	405	445	0.03%	0.004%
65	9.790	2626	2628	2637	rVB2	612	571	0.04%	0.005%
66	9.989	2687	2690	2696	rBV3	415	478	0.03%	0.004%
67	10.054	2703	2710	2715	rBV4	590	853	0.06%	0.008%
68	10.128	2727	2733	2734	rBV4	573	459	0.03%	0.004%
69	10.208	2756	2758	2763	rVB	523	399	0.03%	0.004%
70	10.237	2763	2767	2772	rBV2	469	606	0.04%	0.005%
71	10.317	2787	2792	2795	rBV2	431	470	0.03%	0.004%
72	10.488	2841	2845	2849	rVB3	591	538	0.04%	0.005%
73	10.517	2849	2854	2858	rBV	483	557	0.04%	0.005%
74	10.581	2867	2874	2880	rVB2	503	647	0.04%	0.006%
75	10.626	2884	2888	2891	rVB2	498	380	0.03%	0.003%
76	10.755	2915	2928	2953	rVV	537280	862710	56.94%	7.669%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051094.D
 Acq On : 03 Oct 2022 19:48
 Operator : JC/MD
 Sample : N4854-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.880	2962	2967	2969	rBV2	1028	888	0.06%	0.008%
78	10.896	2969	2972	2978	rVB5	1697	1802	0.12%	0.016%
79	11.031	3007	3014	3017	rBV3	583	701	0.05%	0.006%
80	11.359	3111	3116	3120	rVB2	681	627	0.04%	0.006%
81	11.809	3244	3256	3278	rBV	444845	717991	47.39%	6.383%
82	12.089	3339	3343	3349	rVB2	882	933	0.06%	0.008%
83	12.121	3349	3353	3354	rBV2	654	437	0.03%	0.004%
84	12.192	3360	3375	3398	rBV	517730	858090	56.63%	7.628%
85	12.619	3504	3508	3512	rVV	398	452	0.03%	0.004%
86	12.816	3565	3569	3571	rBV2	667	475	0.03%	0.004%
87	12.835	3571	3575	3577	rBV2	596	417	0.03%	0.004%
88	13.057	3640	3644	3648	rBV2	771	773	0.05%	0.007%
89	13.092	3651	3655	3659	rBV2	614	552	0.04%	0.005%
90	13.160	3672	3676	3682	rBV3	614	847	0.06%	0.008%
91	13.269	3706	3710	3714	rVB3	501	463	0.03%	0.004%
92	13.333	3728	3730	3735	rBV3	461	370	0.02%	0.003%
93	13.388	3742	3747	3750	rBV2	484	540	0.04%	0.005%
94	13.516	3785	3787	3792	rVB2	483	394	0.03%	0.004%
95	13.860	3891	3894	3897	rBV2	805	611	0.04%	0.005%
96	13.928	3912	3915	3920	rBV2	486	487	0.03%	0.004%
97	14.198	3996	3999	4002	rBV2	587	449	0.03%	0.004%
98	14.365	4049	4051	4056	rBV	551	431	0.03%	0.004%
99	14.561	4109	4112	4116	rBV	768	734	0.05%	0.007%
100	15.561	4421	4423	4425	rBV2	741	402	0.03%	0.004%




Sum of corrected areas: 11248856

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051094.D
Acq On : 03 Oct 2022 19:48
Operator : JC/MD
Sample : N4854-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

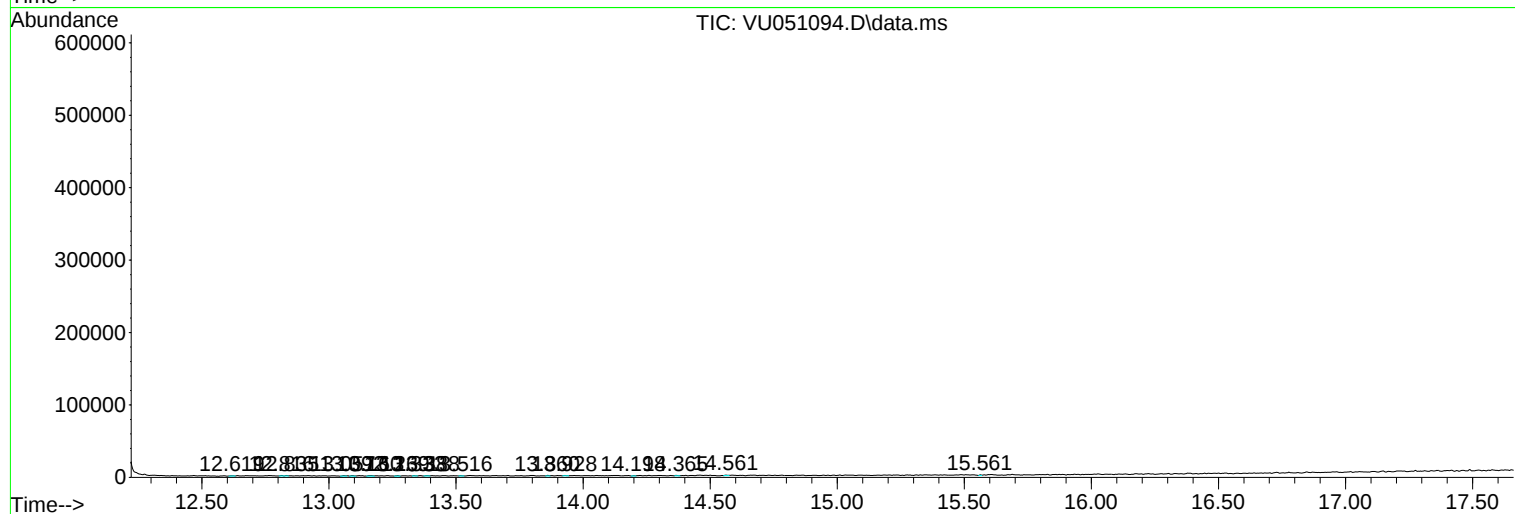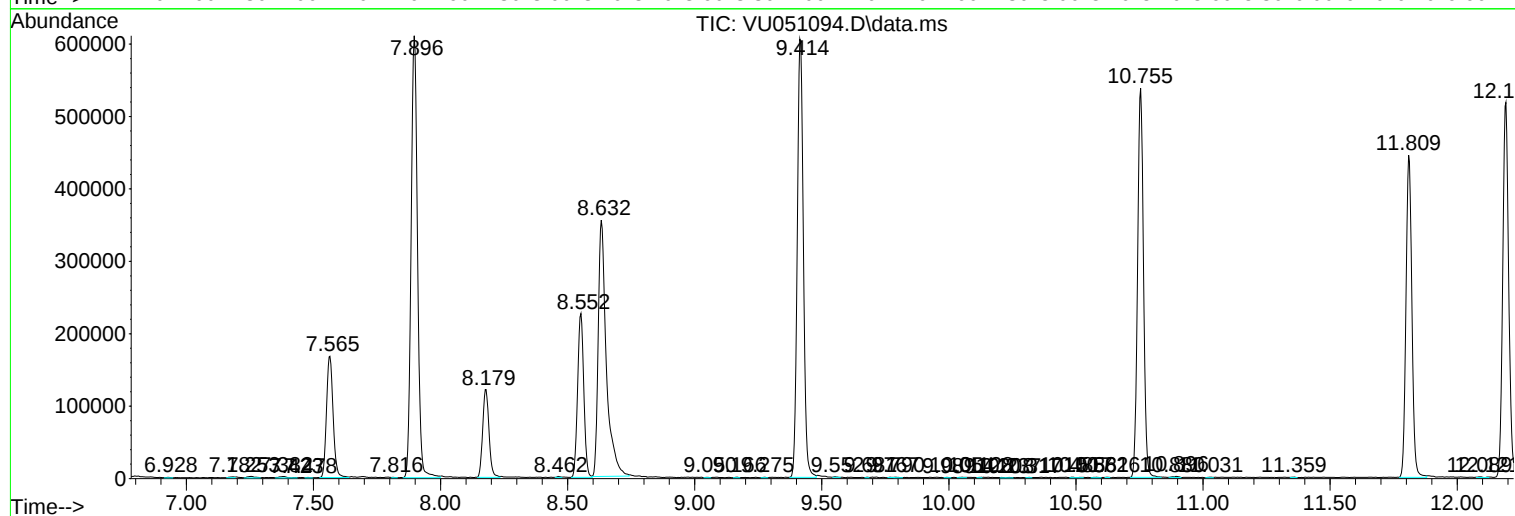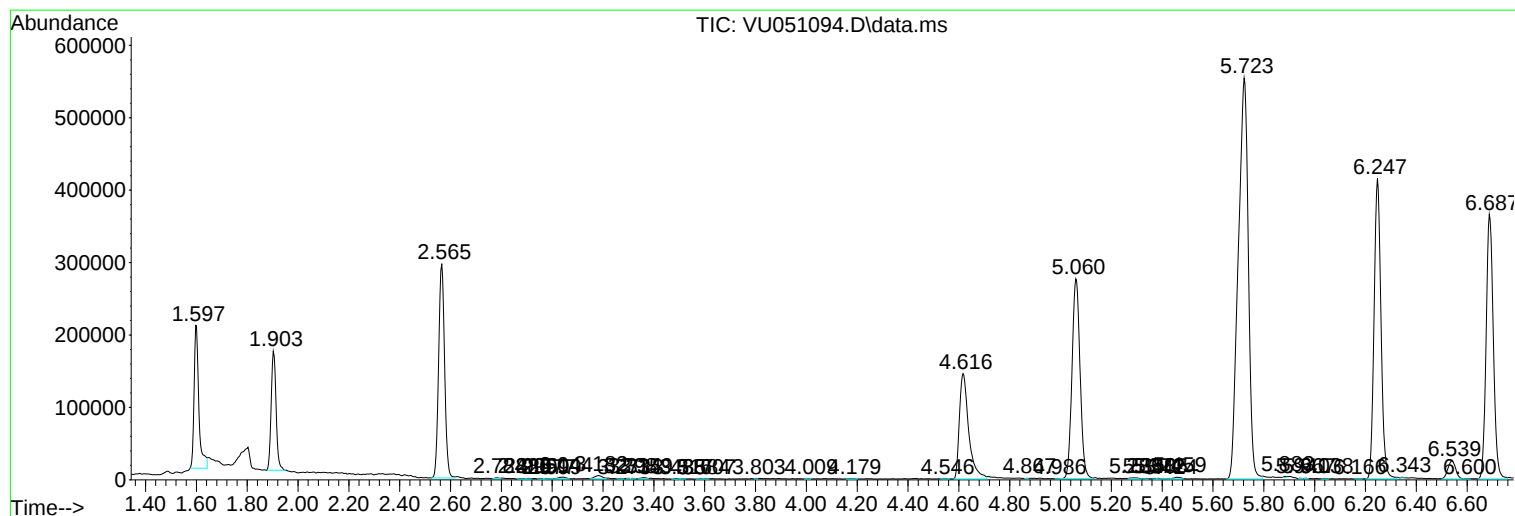

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051094.D
Acq On : 03 Oct 2022 19:48
Operator : JC/MD
Sample : N4854-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051094.D
Acq On : 03 Oct 2022 19:48
Operator : JC/MD
Sample : N4854-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------