

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051095.D
 Acq On : 03 Oct 2022 20:11
 Operator : JC/MD
 Sample : N4854-16 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	39	46	51	rBV5	5738	8817	0.53%	0.069%
2	1.600	74	81	97	rBV	185722	231913	13.95%	1.815%
3	1.903	167	175	190	rVB	158497	216026	12.99%	1.691%
4	2.565	368	381	395	rBV	289981	468194	28.16%	3.665%
5	2.665	408	412	416	rVB3	748	644	0.04%	0.005%
6	2.687	416	419	421	rBV	629	470	0.03%	0.004%
7	2.797	445	453	459	rBV4	1816	2656	0.16%	0.021%
8	2.928	490	494	497	rBV	582	489	0.03%	0.004%
9	2.954	497	502	506	rVV4	857	933	0.06%	0.007%
10	3.044	519	530	541	rBV5	5679	10135	0.61%	0.079%
11	3.176	563	571	586	rVB3	5900	13872	0.83%	0.109%
12	3.301	605	610	613	rVV2	429	391	0.02%	0.003%
13	3.359	613	628	641	rVV5	6226	13982	0.84%	0.109%
14	3.411	641	644	649	rVB	469	416	0.03%	0.003%
15	3.446	649	655	658	rBV2	348	426	0.03%	0.003%
16	3.530	676	681	684	rBV2	391	420	0.03%	0.003%
17	3.681	725	728	732	rBV	407	330	0.02%	0.003%
18	3.719	737	740	743	rBV2	464	297	0.02%	0.002%
19	3.864	780	785	787	rBV2	651	559	0.03%	0.004%
20	3.973	814	819	825	rVB2	437	489	0.03%	0.004%
21	4.491	977	980	987	rVB	523	609	0.04%	0.005%
22	4.616	1005	1019	1045	rBV	150982	385558	23.19%	3.018%
23	4.970	1127	1129	1133	rBV3	680	421	0.03%	0.003%
24	5.060	1140	1157	1182	rBV	277860	615224	37.01%	4.816%
25	5.285	1221	1227	1229	rBV5	1099	1144	0.07%	0.009%
26	5.375	1249	1255	1257	rBV5	966	1142	0.07%	0.009%
27	5.456	1273	1280	1282	rBV4	921	1066	0.06%	0.008%
28	5.568	1312	1315	1319	rVB	441	308	0.02%	0.002%
29	5.607	1319	1327	1331	rBV2	439	675	0.04%	0.005%
30	5.629	1331	1334	1337	rVB2	419	298	0.02%	0.002%
31	5.652	1337	1341	1342	rBV	470	295	0.02%	0.002%
32	5.722	1342	1363	1397	rBV2	554792	1531554	92.13%	11.990%
33	6.102	1475	1481	1484	rBV4	601	600	0.04%	0.005%
34	6.247	1509	1526	1547	rBV	428163	820734	49.37%	6.425%
35	6.398	1569	1573	1576	rBV4	699	516	0.03%	0.004%
36	6.539	1604	1617	1629	rVV4	14571	31855	1.92%	0.249%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051095.D
 Acq On : 03 Oct 2022 20:11
 Operator : JC/MD
 Sample : N4854-16 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.687	1647	1663	1683	rBV	365893	718066	43.19%	5.621%
38	6.896	1726	1728	1734	rVB3	589	481	0.03%	0.004%
39	6.980	1751	1754	1759	rVB2	503	428	0.03%	0.003%
40	7.025	1759	1768	1772	rBV2	598	641	0.04%	0.005%
41	7.108	1784	1794	1804	rVB3	1143	2295	0.14%	0.018%
42	7.189	1809	1819	1827	rBV5	1676	3254	0.20%	0.025%
43	7.256	1837	1840	1841	rBV	584	298	0.02%	0.002%
44	7.385	1873	1880	1883	rVB3	500	546	0.03%	0.004%
45	7.565	1922	1936	1959	rBV	170796	306092	18.41%	2.396%
46	7.751	1990	1994	1997	rBV3	480	451	0.03%	0.004%
47	7.793	2001	2007	2018	rVB7	2668	3802	0.23%	0.030%
48	7.896	2025	2039	2058	rBV	622465	1066357	64.15%	8.348%
49	8.179	2115	2127	2145	rVV	122493	209072	12.58%	1.637%
50	8.401	2189	2196	2205	rVB8	2854	4572	0.28%	0.036%
51	8.449	2206	2211	2213	rBV3	705	567	0.03%	0.004%
52	8.552	2228	2243	2257	rBV	992064	1662396	100.00%	13.014%
53	8.632	2257	2268	2304	rVB3	374431	834774	50.22%	6.535%
54	8.841	2330	2333	2335	rVB4	758	456	0.03%	0.004%
55	8.861	2336	2339	2341	rBV3	522	348	0.02%	0.003%
56	8.963	2367	2371	2373	rBV4	476	395	0.02%	0.003%
57	9.041	2393	2395	2398	rBV2	453	310	0.02%	0.002%
58	9.121	2414	2420	2423	rBV2	487	562	0.03%	0.004%
59	9.182	2435	2439	2444	rVB3	366	339	0.02%	0.003%
60	9.298	2472	2475	2479	rVB	595	473	0.03%	0.004%
61	9.417	2496	2512	2532	rBV	632713	1061299	63.84%	8.308%
62	9.568	2553	2559	2568	rVB4	2994	4928	0.30%	0.039%
63	9.636	2576	2580	2583	rBV2	501	500	0.03%	0.004%
64	9.697	2590	2599	2605	rBV4	2136	2819	0.17%	0.022%
65	9.947	2674	2677	2682	rVB	449	348	0.02%	0.003%
66	10.002	2691	2694	2701	rVB3	520	580	0.03%	0.005%
67	10.041	2703	2706	2713	rVB3	716	657	0.04%	0.005%
68	10.079	2713	2718	2719	rBV2	555	486	0.03%	0.004%
69	10.102	2719	2725	2729	rBV5	2235	2778	0.17%	0.022%
70	10.230	2763	2765	2770	rVB	501	301	0.02%	0.002%
71	10.439	2827	2830	2835	rVB2	463	370	0.02%	0.003%
72	10.484	2835	2844	2852	rVB5	2153	3318	0.20%	0.026%
73	10.520	2852	2855	2859	rBV2	445	402	0.02%	0.003%
74	10.754	2914	2928	2944	rBV	530989	866877	52.15%	6.786%
75	11.021	3007	3011	3014	rBV2	375	306	0.02%	0.002%
76	11.089	3027	3032	3038	rBV5	886	1114	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051095.D
 Acq On : 03 Oct 2022 20:11
 Operator : JC/MD
 Sample : N4854-16 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.143	3045	3049	3056	rBV2	620	581	0.03%	0.005%
78	11.198	3061	3066	3069	rBV	507	396	0.02%	0.003%
79	11.465	3144	3149	3150	rBV3	1299	1025	0.06%	0.008%
80	11.745	3232	3236	3244	rVB4	1672	2138	0.13%	0.017%
81	11.809	3244	3256	3287	rBV	469979	764064	45.96%	5.981%
82	11.999	3313	3315	3319	rVB	579	307	0.02%	0.002%
83	12.192	3362	3375	3395	rBV	525235	867943	52.21%	6.795%
84	12.378	3430	3433	3437	rBV3	408	335	0.02%	0.003%
85	12.414	3441	3444	3446	rVB3	697	413	0.02%	0.003%
86	12.430	3446	3449	3456	rBV3	511	596	0.04%	0.005%
87	12.523	3475	3478	3483	rVB3	754	668	0.04%	0.005%
88	12.838	3572	3576	3578	rBV2	438	401	0.02%	0.003%
89	12.989	3621	3623	3626	rVB3	562	306	0.02%	0.002%
90	13.114	3659	3662	3666	rBV3	526	366	0.02%	0.003%
91	13.137	3666	3669	3671	rBV	492	349	0.02%	0.003%
92	13.227	3691	3697	3705	rVB5	1598	1994	0.12%	0.016%
93	13.397	3745	3750	3753	rBV3	545	551	0.03%	0.004%
94	13.706	3843	3846	3848	rBV2	474	364	0.02%	0.003%
95	13.783	3867	3870	3872	rBV4	490	303	0.02%	0.002%
96	13.979	3928	3931	3935	rBV3	459	384	0.02%	0.003%
97	14.002	3935	3938	3940	rBV	592	388	0.02%	0.003%
98	14.536	4100	4104	4109	rBV	726	863	0.05%	0.007%
99	15.028	4250	4257	4259	rBV4	720	993	0.06%	0.008%
100	16.217	4625	4627	4630	rBV4	1162	822	0.05%	0.006%




Sum of corrected areas: 12774066

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051095.D
Acq On : 03 Oct 2022 20:11
Operator : JC/MD
Sample : N4854-16 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

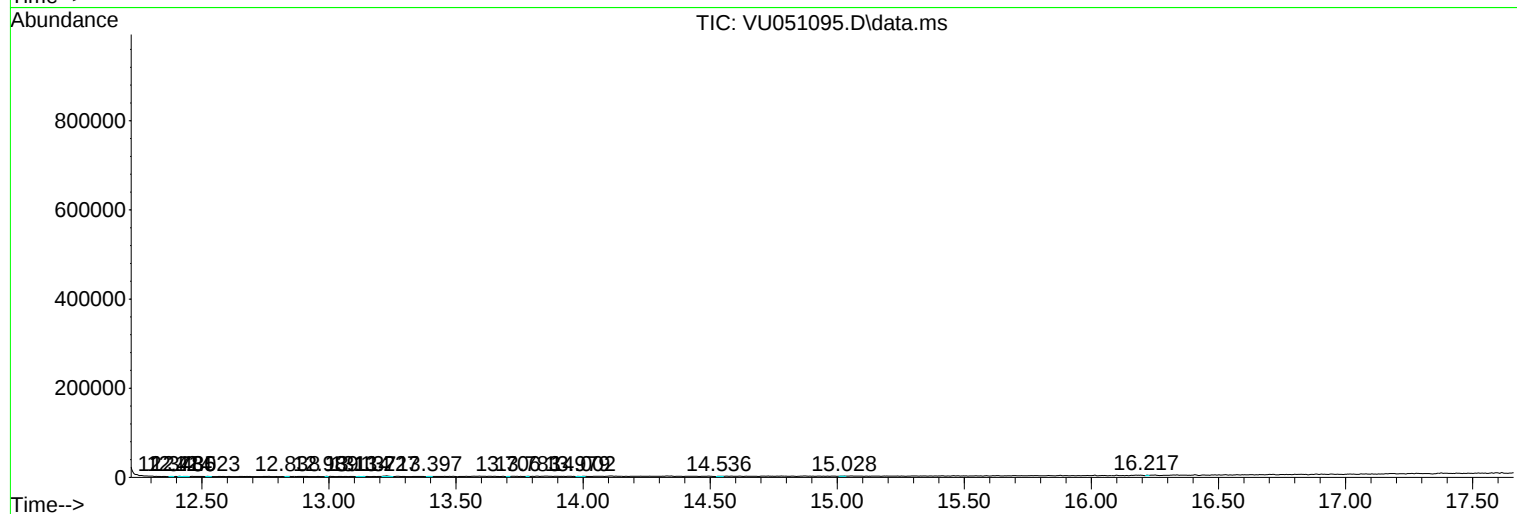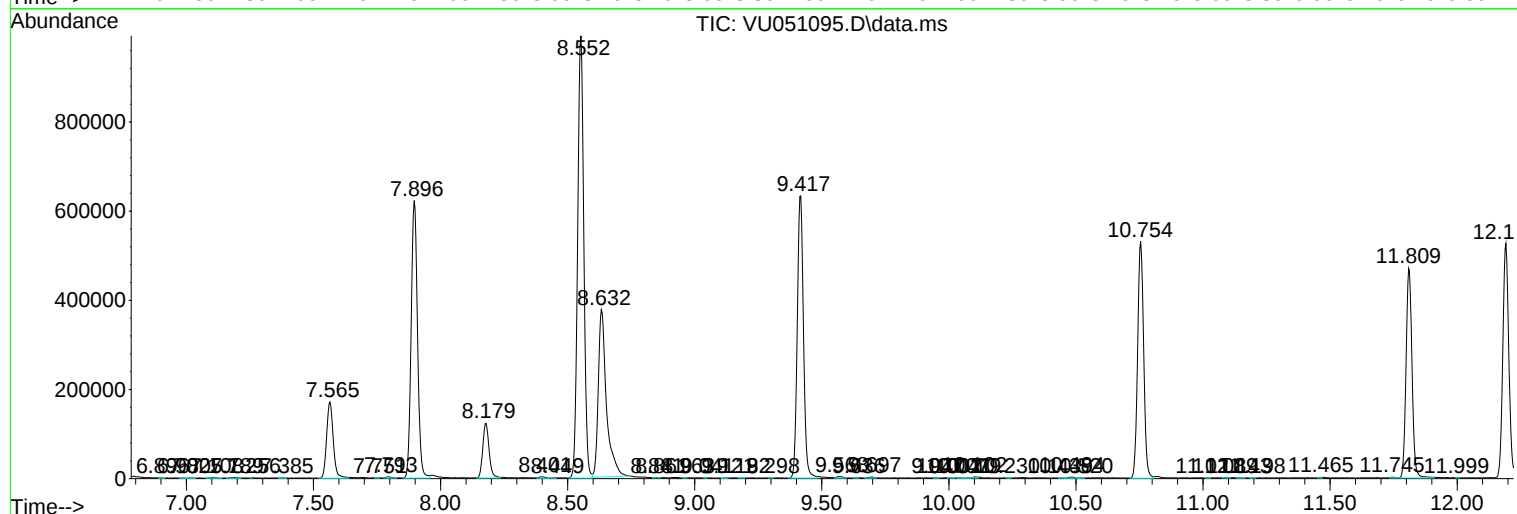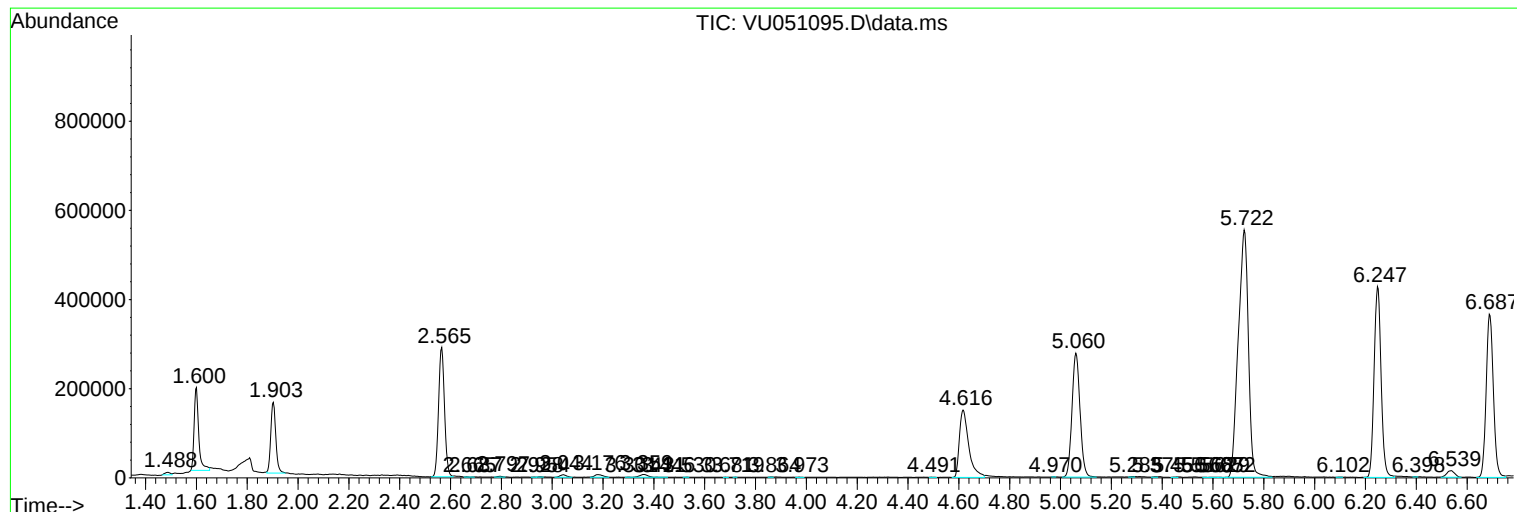

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051095.D
Acq On : 03 Oct 2022 20:11
Operator : JC/MD
Sample : N4854-16 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051095.D
Acq On : 03 Oct 2022 20:11
Operator : JC/MD
Sample : N4854-16 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc