

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051096.D
 Acq On : 03 Oct 2022 20:35
 Operator : JC/MD
 Sample : N4880-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.357	3	5	12	rVB	9375	7313	0.46%	0.065%
2	1.598	72	80	99	rBV	205308	265334	16.87%	2.346%
3	1.903	167	175	198	rVB	169838	236016	15.00%	2.087%
4	2.566	367	381	394	rBV	299511	489220	31.10%	4.326%
5	2.765	440	443	445	rVB2	596	330	0.02%	0.003%
6	2.784	445	449	456	rBV3	764	794	0.05%	0.007%
7	2.836	461	465	466	rBV3	676	391	0.02%	0.003%
8	2.852	466	470	471	rBV2	612	455	0.03%	0.004%
9	2.913	487	489	494	rBV2	422	318	0.02%	0.003%
10	3.006	515	518	523	rBV3	430	464	0.03%	0.004%
11	3.045	523	530	542	rVB3	1837	3059	0.19%	0.027%
12	3.125	552	555	559	rVB4	489	355	0.02%	0.003%
13	3.176	564	571	572	rBV3	1320	1370	0.09%	0.012%
14	3.238	585	590	593	rBV2	523	460	0.03%	0.004%
15	3.260	593	597	602	rVB2	404	377	0.02%	0.003%
16	3.565	688	692	694	rBV3	493	421	0.03%	0.004%
17	3.643	711	716	723	rVB2	339	353	0.02%	0.003%
18	3.778	755	758	762	rVB3	503	398	0.03%	0.004%
19	3.829	772	774	781	rVB3	479	436	0.03%	0.004%
20	3.903	790	797	799	rBV3	448	455	0.03%	0.004%
21	4.006	823	829	834	rBV2	429	410	0.03%	0.004%
22	4.141	865	871	874	rVB2	562	481	0.03%	0.004%
23	4.340	927	933	935	rBV2	519	513	0.03%	0.005%
24	4.453	965	968	972	rBV3	523	425	0.03%	0.004%
25	4.514	983	987	991	rVV2	403	404	0.03%	0.004%
26	4.617	1006	1019	1059	rBV	150090	380232	24.17%	3.362%
27	4.877	1097	1100	1103	rVB2	1151	675	0.04%	0.006%
28	4.938	1116	1119	1122	rBV2	494	367	0.02%	0.003%
29	5.061	1141	1157	1179	rVV	292515	646327	41.08%	5.716%
30	5.279	1220	1225	1228	rBV3	829	904	0.06%	0.008%
31	5.340	1239	1244	1246	rBV4	461	414	0.03%	0.004%
32	5.437	1270	1274	1278	rBV3	815	696	0.04%	0.006%
33	5.479	1284	1287	1295	rVB2	424	395	0.03%	0.003%
34	5.546	1304	1308	1314	rVB2	292	327	0.02%	0.003%
35	5.723	1339	1363	1396	rBV2	573155	1573219	100.00%	13.912%
36	6.041	1457	1462	1465	rVB5	504	430	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051096.D
 Acq On : 03 Oct 2022 20:35
 Operator : JC/MD
 Sample : N4880-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.080	1471	1474	1477	rVB	510	376	0.02%	0.003%
38	6.115	1477	1485	1488	rBV2	542	720	0.05%	0.006%
39	6.157	1495	1498	1501	rVB2	611	432	0.03%	0.004%
40	6.186	1501	1507	1511	rBV3	499	478	0.03%	0.004%
41	6.247	1511	1526	1550	rBV	429108	816658	51.91%	7.222%
42	6.401	1571	1574	1578	rBV3	532	416	0.03%	0.004%
43	6.466	1592	1594	1600	rVB3	824	601	0.04%	0.005%
44	6.530	1604	1614	1626	rVB8	7489	15325	0.97%	0.136%
45	6.604	1631	1637	1641	rBV	908	697	0.04%	0.006%
46	6.688	1647	1663	1683	rBV	377065	742632	47.20%	6.567%
47	7.176	1810	1815	1823	rBV4	939	1544	0.10%	0.014%
48	7.231	1829	1832	1835	rBV2	653	409	0.03%	0.004%
49	7.276	1844	1846	1851	rVB2	435	320	0.02%	0.003%
50	7.334	1860	1864	1873	rVB2	601	779	0.05%	0.007%
51	7.379	1873	1878	1884	rBV2	717	736	0.05%	0.007%
52	7.440	1891	1897	1899	rBV	473	468	0.03%	0.004%
53	7.562	1921	1935	1956	rBV	174943	312822	19.88%	2.766%
54	7.726	1984	1986	1991	rVB2	771	556	0.04%	0.005%
55	7.800	2007	2009	2013	rBV	482	402	0.03%	0.004%
56	7.896	2025	2039	2076	rBV	623040	1105795	70.29%	9.779%
57	8.176	2115	2126	2142	rBV	125119	213956	13.60%	1.892%
58	8.302	2162	2165	2168	rBV3	537	384	0.02%	0.003%
59	8.466	2213	2216	2225	rVB4	927	1224	0.08%	0.011%
60	8.552	2233	2243	2254	rVB2	24263	40714	2.59%	0.360%
61	8.633	2255	2268	2305	rBV2	372743	835365	53.10%	7.387%
62	9.067	2400	2403	2408	rVB2	572	451	0.03%	0.004%
63	9.314	2477	2480	2483	rVB2	729	493	0.03%	0.004%
64	9.347	2483	2490	2494	rBV2	654	699	0.04%	0.006%
65	9.414	2494	2511	2533	rBV	625820	1042754	66.28%	9.221%
66	9.620	2569	2575	2578	rBV5	414	528	0.03%	0.005%
67	9.694	2594	2598	2606	rVB4	910	1109	0.07%	0.010%
68	9.912	2662	2666	2671	rBV2	446	471	0.03%	0.004%
69	10.202	2753	2756	2760	rBV2	461	388	0.02%	0.003%
70	10.279	2776	2780	2783	rVB	503	394	0.03%	0.003%
71	10.347	2797	2801	2804	rBV	1021	883	0.06%	0.008%
72	10.404	2815	2819	2824	rBV2	389	456	0.03%	0.004%
73	10.433	2825	2828	2831	rVB2	438	332	0.02%	0.003%
74	10.601	2876	2880	2884	rVB2	565	408	0.03%	0.004%
75	10.623	2884	2887	2890	rBV	598	513	0.03%	0.005%
76	10.755	2914	2928	2949	rBV	550501	885232	56.27%	7.828%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051096.D
 Acq On : 03 Oct 2022 20:35
 Operator : JC/MD
 Sample : N4880-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.887	2966	2969	2972	rBV3	564	420	0.03%	0.004%
78	11.076	3023	3028	3031	rBV2	513	566	0.04%	0.005%
79	11.112	3036	3039	3050	rVB5	828	958	0.06%	0.008%
80	11.440	3138	3141	3144	rBV	470	425	0.03%	0.004%
81	11.501	3156	3160	3165	rBV2	720	846	0.05%	0.007%
82	11.584	3182	3186	3190	rBV2	369	344	0.02%	0.003%
83	11.633	3196	3201	3202	rBV	500	367	0.02%	0.003%
84	11.691	3212	3219	3227	rBV5	2479	3433	0.22%	0.030%
85	11.810	3243	3256	3281	rBV	462895	747944	47.54%	6.614%
86	12.067	3332	3336	3337	rBV3	1779	1267	0.08%	0.011%
87	12.105	3346	3348	3353	rBV3	424	378	0.02%	0.003%
88	12.189	3362	3374	3400	rBV	539874	896443	56.98%	7.927%
89	12.896	3588	3594	3604	rVB5	2884	3831	0.24%	0.034%
90	13.002	3621	3627	3630	rBV2	605	768	0.05%	0.007%
91	13.035	3634	3637	3642	rVV2	638	660	0.04%	0.006%
92	13.070	3642	3648	3651	rBV4	917	890	0.06%	0.008%
93	13.272	3708	3711	3717	rBV3	481	464	0.03%	0.004%
94	13.337	3728	3731	3733	rVB	700	361	0.02%	0.003%
95	13.887	3899	3902	3907	rBV3	416	499	0.03%	0.004%
96	14.687	4148	4151	4152	rBV	672	398	0.03%	0.004%
97	14.925	4222	4225	4226	rBV	588	363	0.02%	0.003%
98	15.173	4299	4302	4309	rVB2	1371	1373	0.09%	0.012%
99	15.343	4349	4355	4357	rBV5	964	1151	0.07%	0.010%
100	15.536	4413	4415	4420	rBV3	749	585	0.04%	0.005%




Sum of corrected areas: 11308192

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051096.D
Acq On : 03 Oct 2022 20:35
Operator : JC/MD
Sample : N4880-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

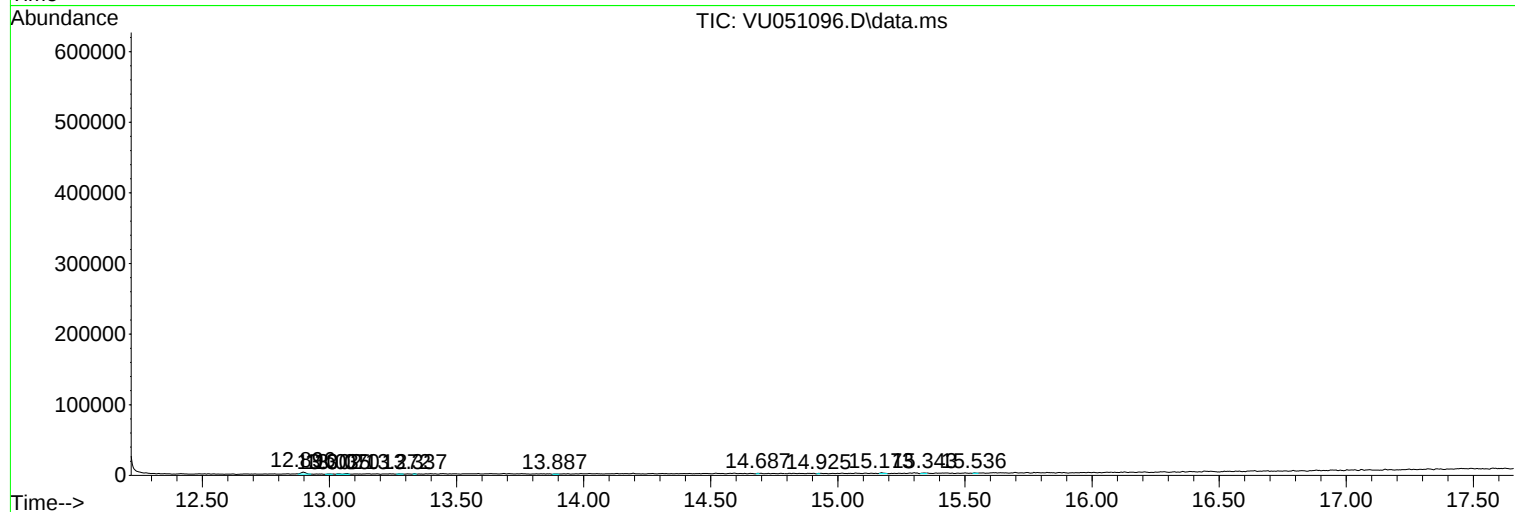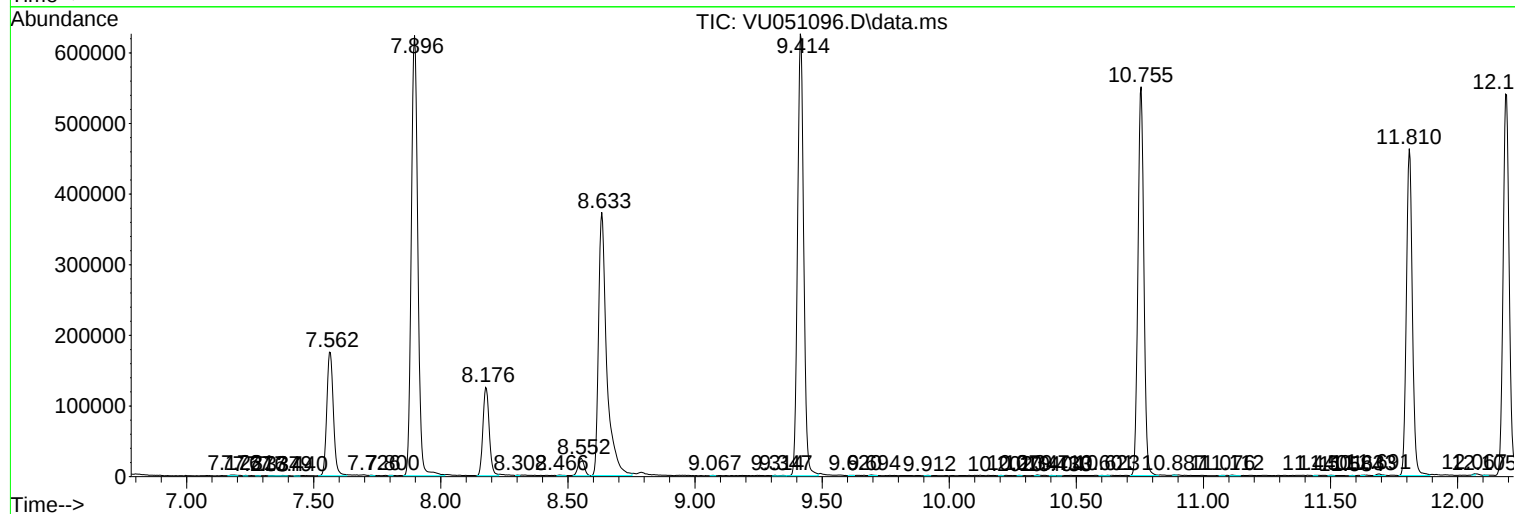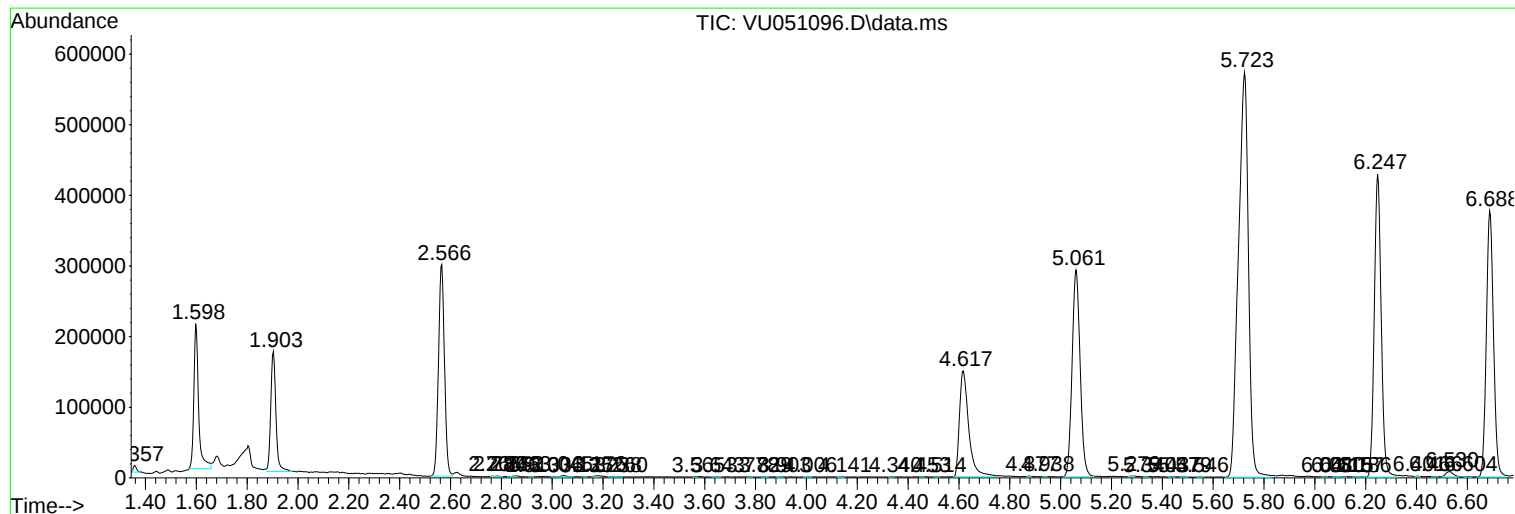

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051096.D
Acq On : 03 Oct 2022 20:35
Operator : JC/MD
Sample : N4880-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051096.D
Acq On : 03 Oct 2022 20:35
Operator : JC/MD
Sample : N4880-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc