

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051271.D
 Acq On : 08 Oct 2022 14:51
 Operator : JC/MD
 Sample : N5049-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BT5

Manual IntegrationsAPPROVED

Quant Time: Oct 08 23:50:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 08 05:40:36 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/10/2022
 Supervised By :Mahesh Dadoda 10/10/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	169354	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	194718	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	70529	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	56212	4.115	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	82.200%	
7) Chloroethane-d5	1.912	69	55955	4.767	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.400%	
11) 1,1-Dichloroethene-d2	2.562	65	22206	4.112	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	82.200%	
20) 2-Butanone-d5	4.639	46	173058	57.539	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	115.080%	
24) Chloroform-d	5.060	84	125766	4.938	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.800%	
26) 1,2-Dichloroethane-d4	5.700	65	69008	5.254	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.000%	
32) Benzene-d6	5.726	84	225840	4.216	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.400%	
36) 1,2-Dichloropropane-d6	6.690	67	83763	4.604	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	92.000%	
41) Toluene-d8	7.896	98	164508	3.433	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	68.600%#	
43) trans-1,3-Dichloroprop...	8.182	79	23665	3.959	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	79.200%	
46) 2-Hexanone-d5	8.636	63	83252	41.329	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	82.660%	
56) 1,1,2,2-Tetrachloroeth...	10.754	84	70549	4.855	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	97.000%	
66) 1,2-Dichlorobenzene-d4	12.192	152	60826	4.962	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	99.200%	
Target Compounds					Qvalue	
13) Acetone	2.658	43	11991m	5.316	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051271.D
Acq On : 08 Oct 2022 14:51
Operator : JC/MD
Sample : N5049-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 63 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT5

Manual IntegrationsAPPROVED

Quant Time: Oct 08 23:50:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 08 05:40:36 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/10/2022

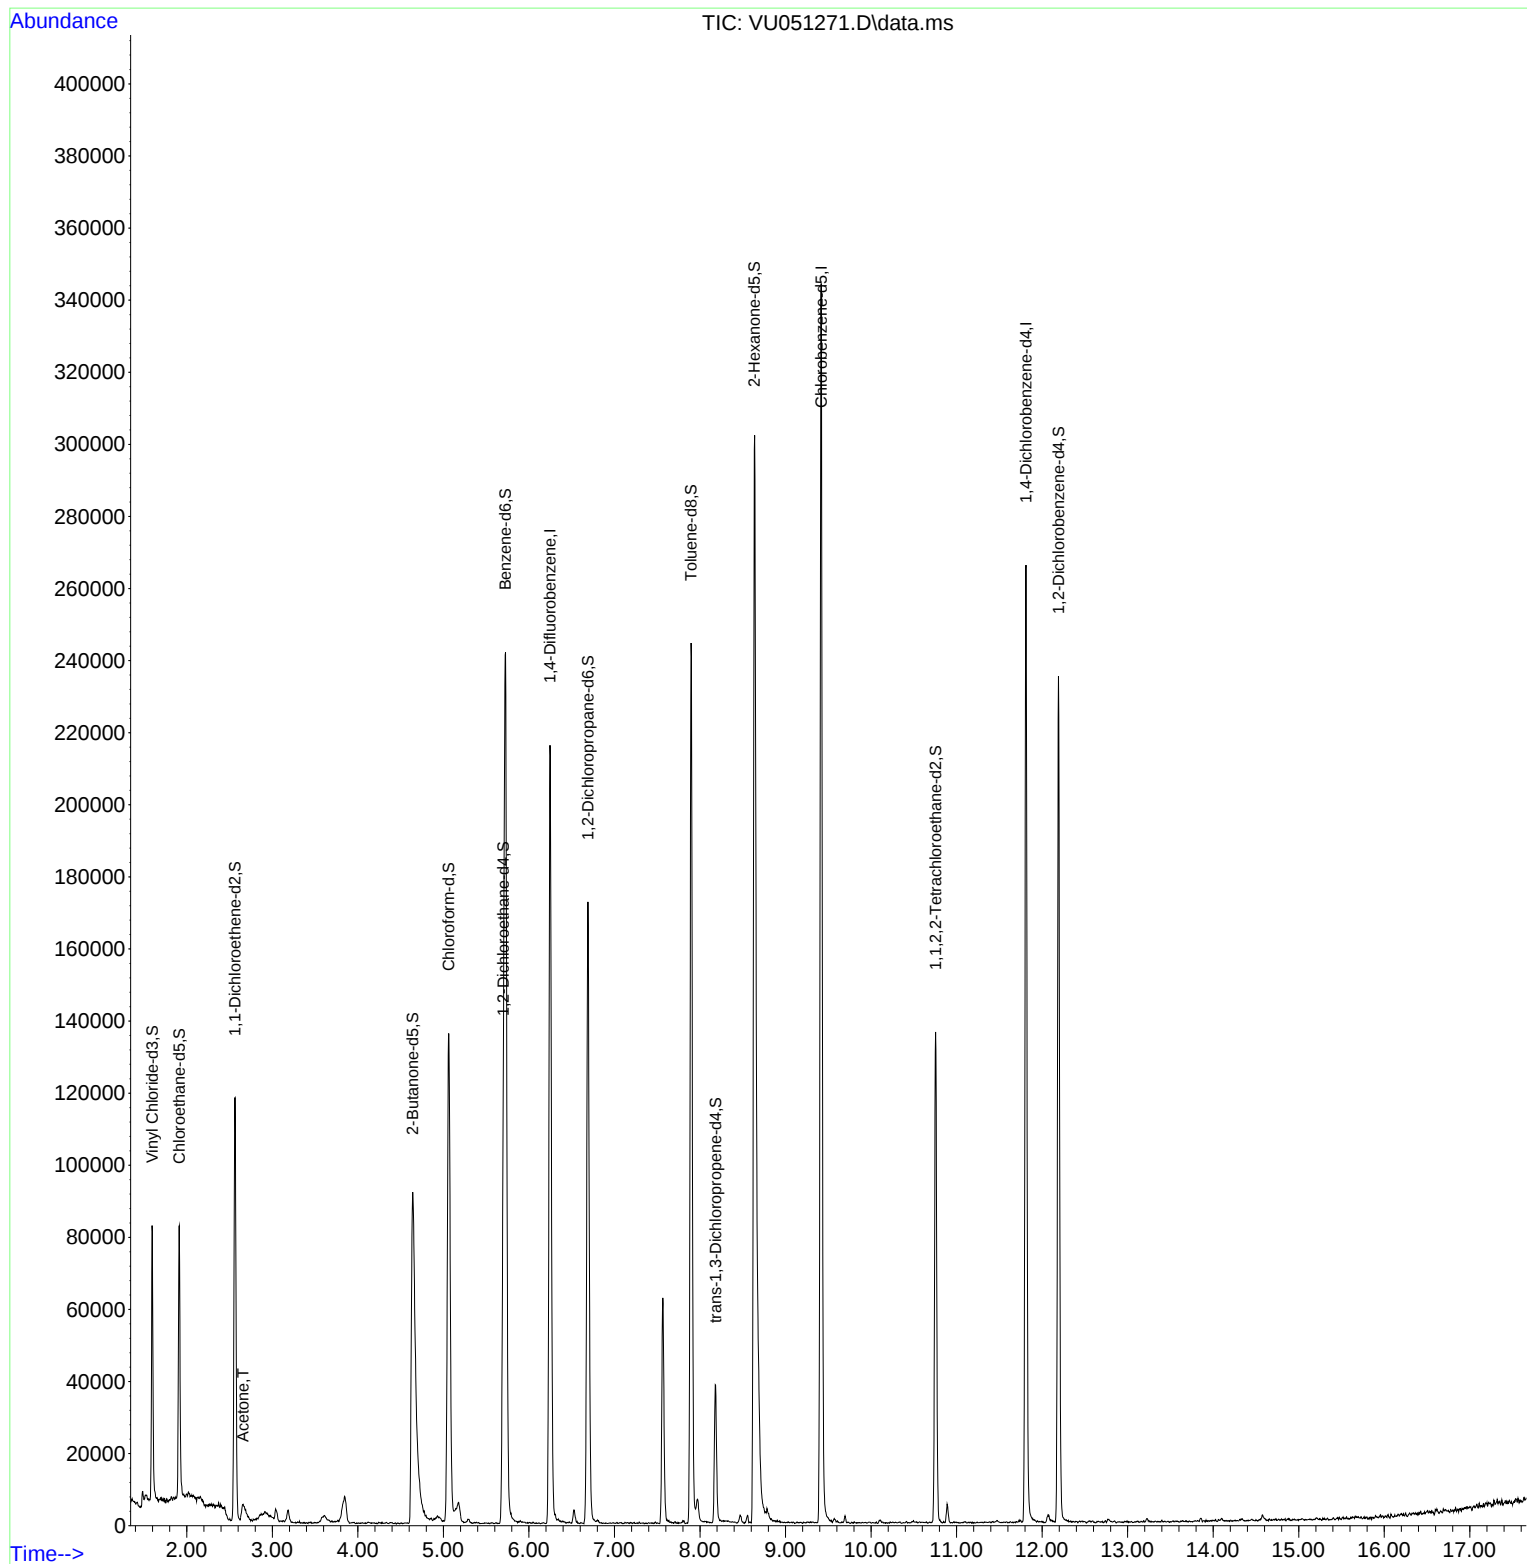




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051271.D
 Acq On : 08 Oct 2022 14:51
 Operator : JC/MD
 Sample : N5049-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BT5

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 10/10/2022
 Supervised By :Mahesh Dadoda 10/10/2022

Quant Time: Oct 08 23:50:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 08 05:40:36 2022
 Response via : Initial Calibration

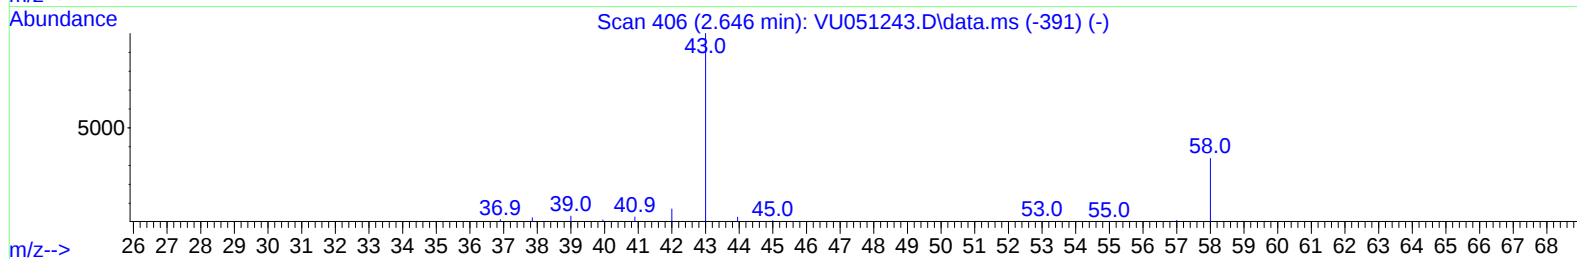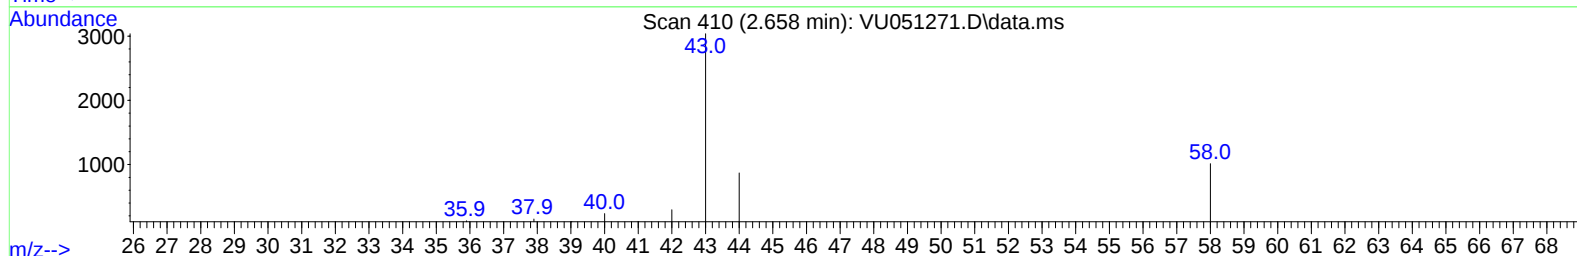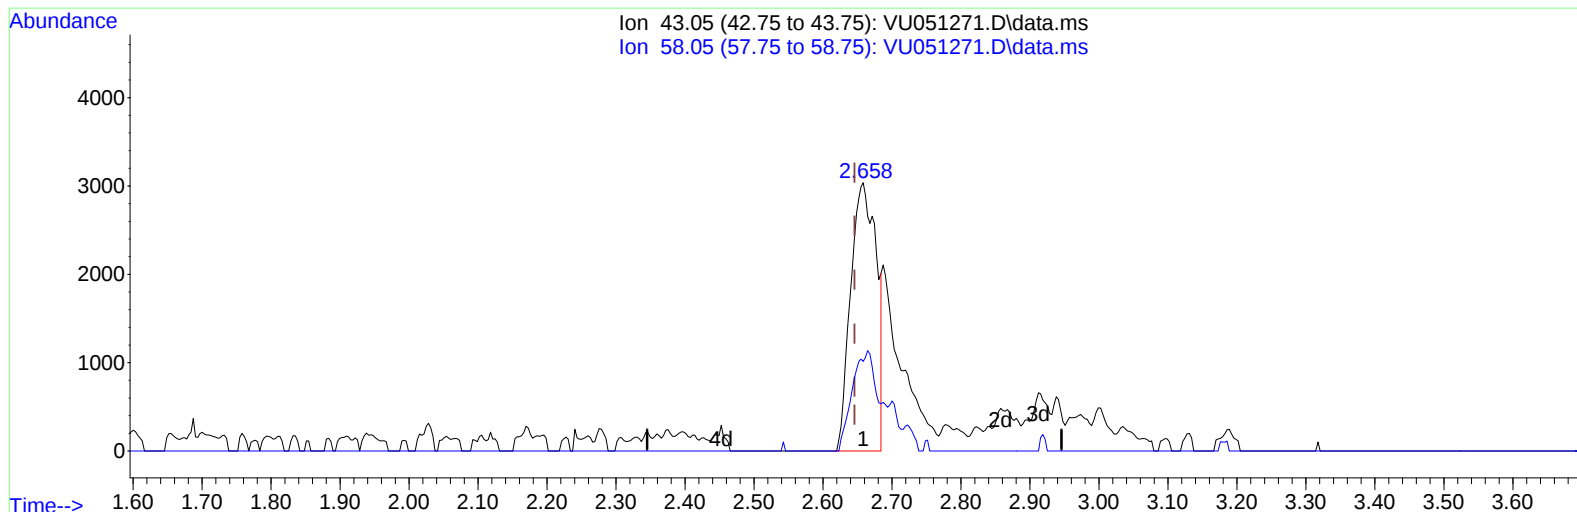

TIC: VU051271.D\data.ms

(13) Acetone (T)

2.658min (+ 0.013) 3.48 ug/L

response 7852

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.40	38.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051271.D
 Acq On : 08 Oct 2022 14:51
 Operator : JC/MD
 Sample : N5049-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BT5

Manual IntegrationsAPPROVED

Quant Time: Oct 08 23:50:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 08 05:40:36 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/10/2022
 Supervised By :Mahesh Dadoda 10/10/2022

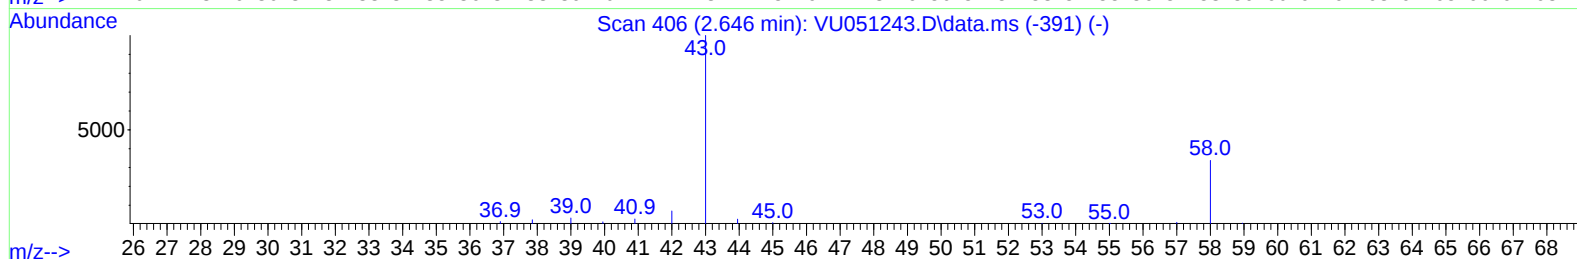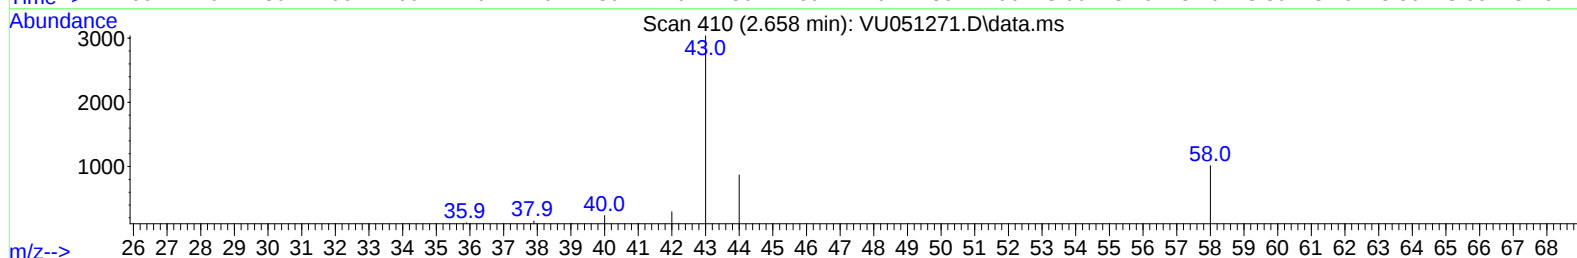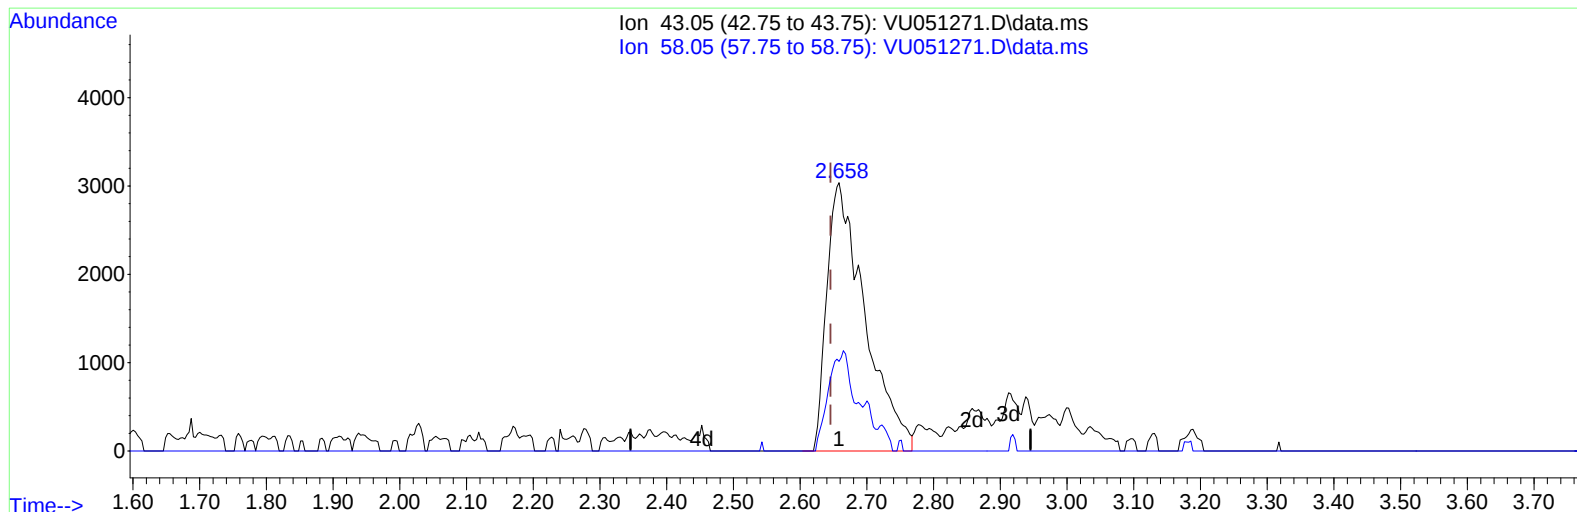

TIC: VU051271.D\data.ms

(13) Acetone (T)

2.658min (+ 0.013) 5.32 ug/L m

response 11991

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.40	24.92
0.00	0.00	0.00
0.00	0.00	0.00