

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051221.D
 Acq On : 07 Oct 2022 16:29
 Operator : JC/MD
 Sample : N4866-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Oct 08 04:26:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 08 00:50:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	174559	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	191448	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	69685	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	69851	4.961	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	99.200%	
7) Chloroethane-d5	1.909	69	62883	5.198	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	104.000%	
11) 1,1-Dichloroethene-d2	2.562	65	26706	4.798	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	96.000%	
20) 2-Butanone-d5	4.642	46	188768	60.891	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	121.780%	
24) Chloroform-d	5.063	84	140228	5.342	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	106.800%	
26) 1,2-Dichloroethane-d4	5.703	65	74938	5.535	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	110.800%	
32) Benzene-d6	5.726	84	264112	5.015	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.200%	
36) 1,2-Dichloropropane-d6	6.690	67	93400	5.222	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.400%	
41) Toluene-d8	7.896	98	204530	4.341	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.800%	
43) trans-1,3-Dichloroprop...	8.179	79	27775	4.726	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.600%	
46) 2-Hexanone-d5	8.636	63	101274	51.134	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	102.260%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	73944	5.175	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	103.600%	
66) 1,2-Dichlorobenzene-d4	12.195	152	67842	5.601	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	112.000%	
Target Compounds						
16) Methylene chloride	3.041	84	6426	0.342	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051221.D
Acq On : 07 Oct 2022 16:29
Operator : JC/MD
Sample : N4866-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Time: Oct 08 04:26:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 08 00:50:53 2022
Response via : Initial Calibration

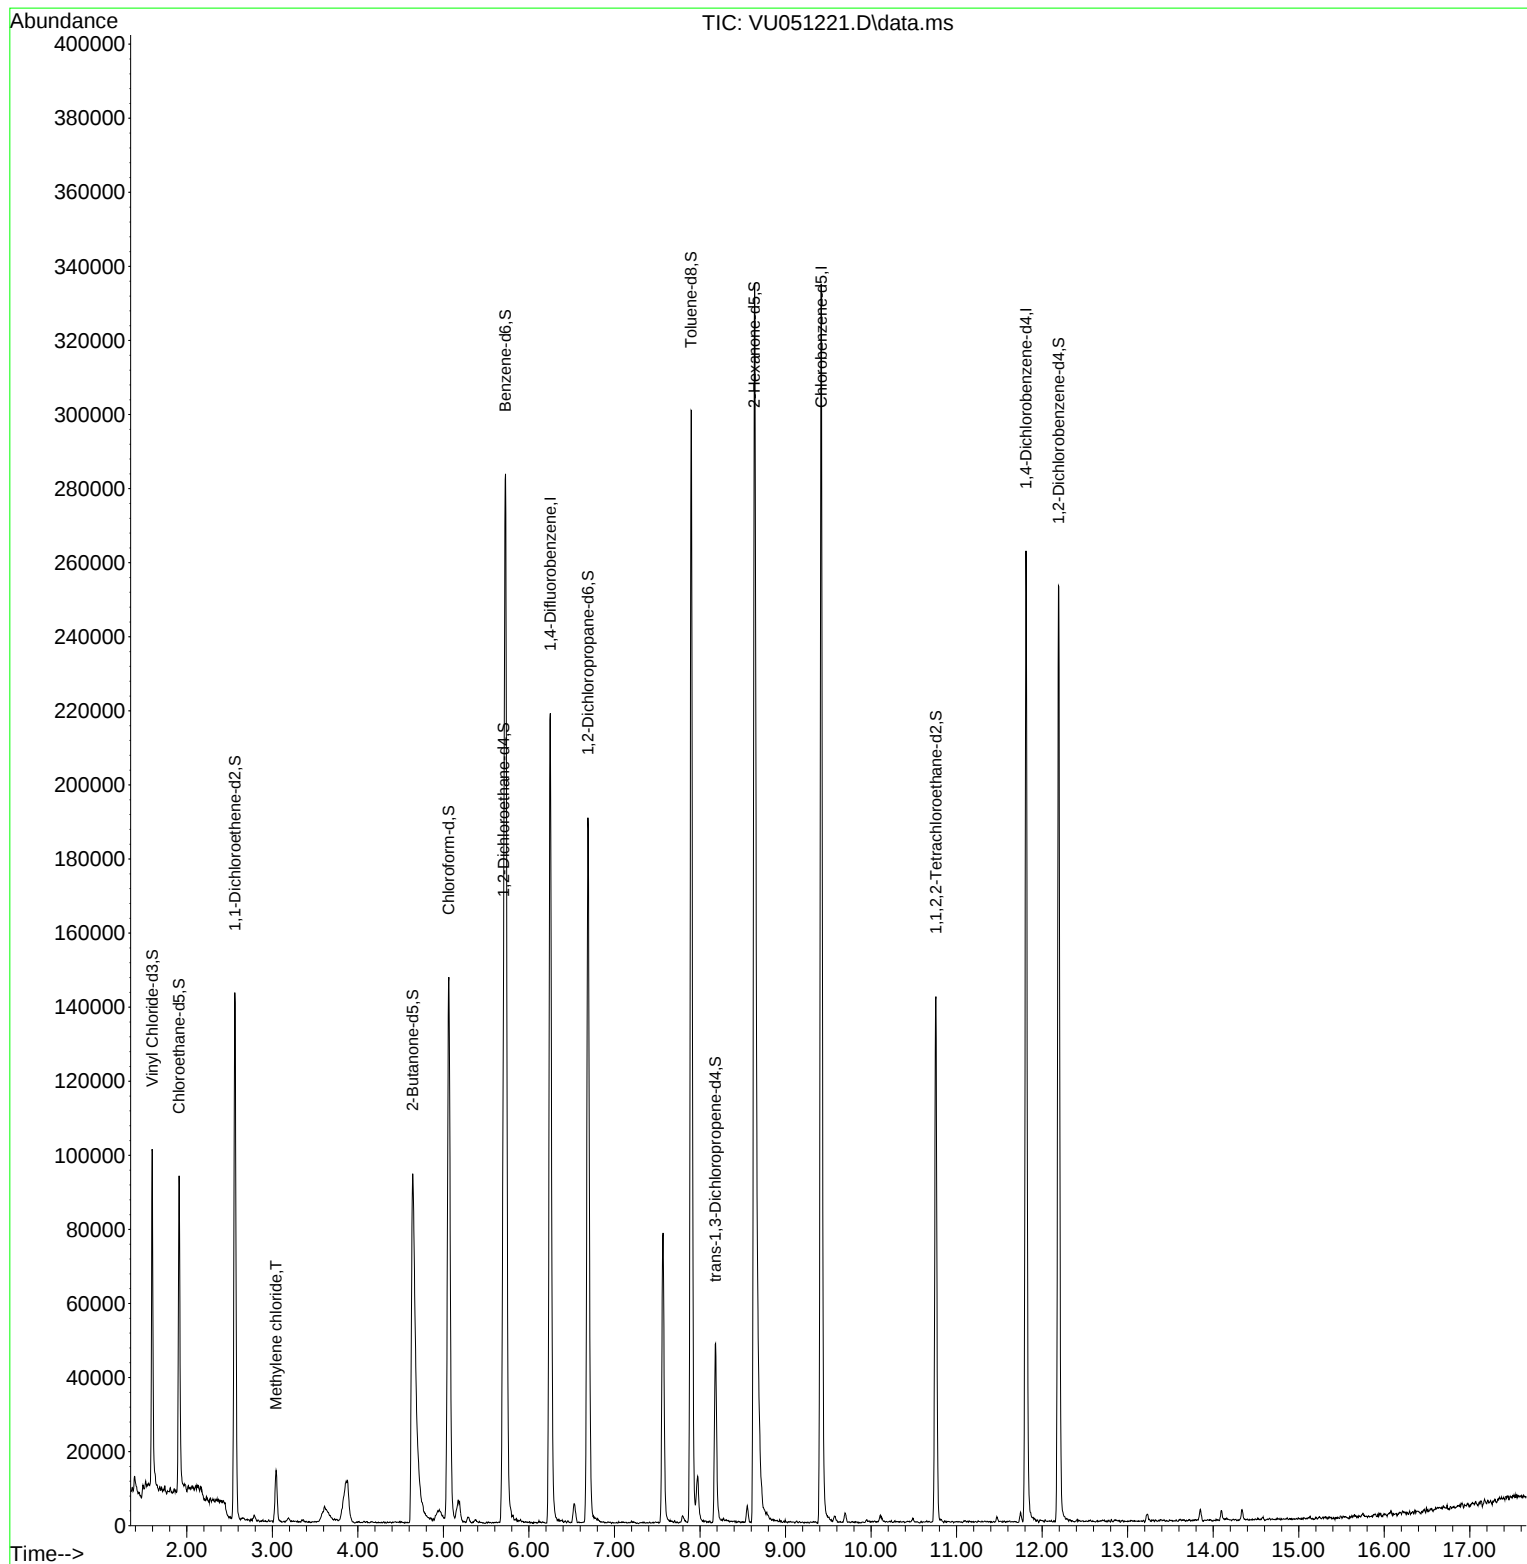

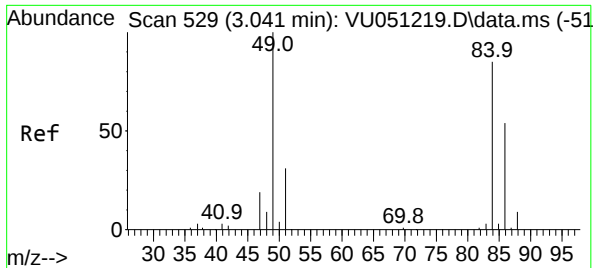

#16
Methylene chloride
Concen: 0.342 ug/L
RT: 3.041 min Scan# 51
Delta R.T. -0.000 min
Lab File: VU051221.D
Acq: 07 Oct 2022 16:29

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	6426
Ion	Ratio	Lower	Upper
84	100		
86	73.5	46.5	86.3
49	122.0	81.3	151.1

