

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051238.D
 Acq On : 07 Oct 2022 23:31
 Operator : JC/MD
 Sample : N4900-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXFS8

Quant Time: Oct 08 04:30:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 08 00:50:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	124239	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	143037	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	47427	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	58177	5.805	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	116.200%
7) Chloroethane-d5	1.909	69	56952	6.614	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	132.200%#
11) 1,1-Dichloroethene-d2	2.562	65	22553	5.693	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	113.800%
20) 2-Butanone-d5	4.620	46	159771	72.411	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	144.820%#
24) Chloroform-d	5.064	84	129817	6.948	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	139.000%#
26) 1,2-Dichloroethane-d4	5.700	65	70747	7.342	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	146.800%#
32) Benzene-d6	5.726	84	227669	5.786	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.800%
36) 1,2-Dichloropropane-d6	6.690	67	83500	6.248	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	125.000%
41) Toluene-d8	7.896	98	169657	4.819	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.400%
43) trans-1,3-Dichloroprop...	8.179	79	24315	5.538	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	110.800%
46) 2-Hexanone-d5	8.633	63	83296	56.291	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	112.580%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	72587	6.800	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	136.000%#
66) 1,2-Dichlorobenzene-d4	12.192	152	61377	7.446	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	149.000%#
Target Compounds					Qvalue	
13) Acetone	2.626	43	6167	3.727	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051238.D
Acq On : 07 Oct 2022 23:31
Operator : JC/MD
Sample : N4900-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXFS8

Quant Time: Oct 08 04:30:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 08 00:50:53 2022
Response via : Initial Calibration

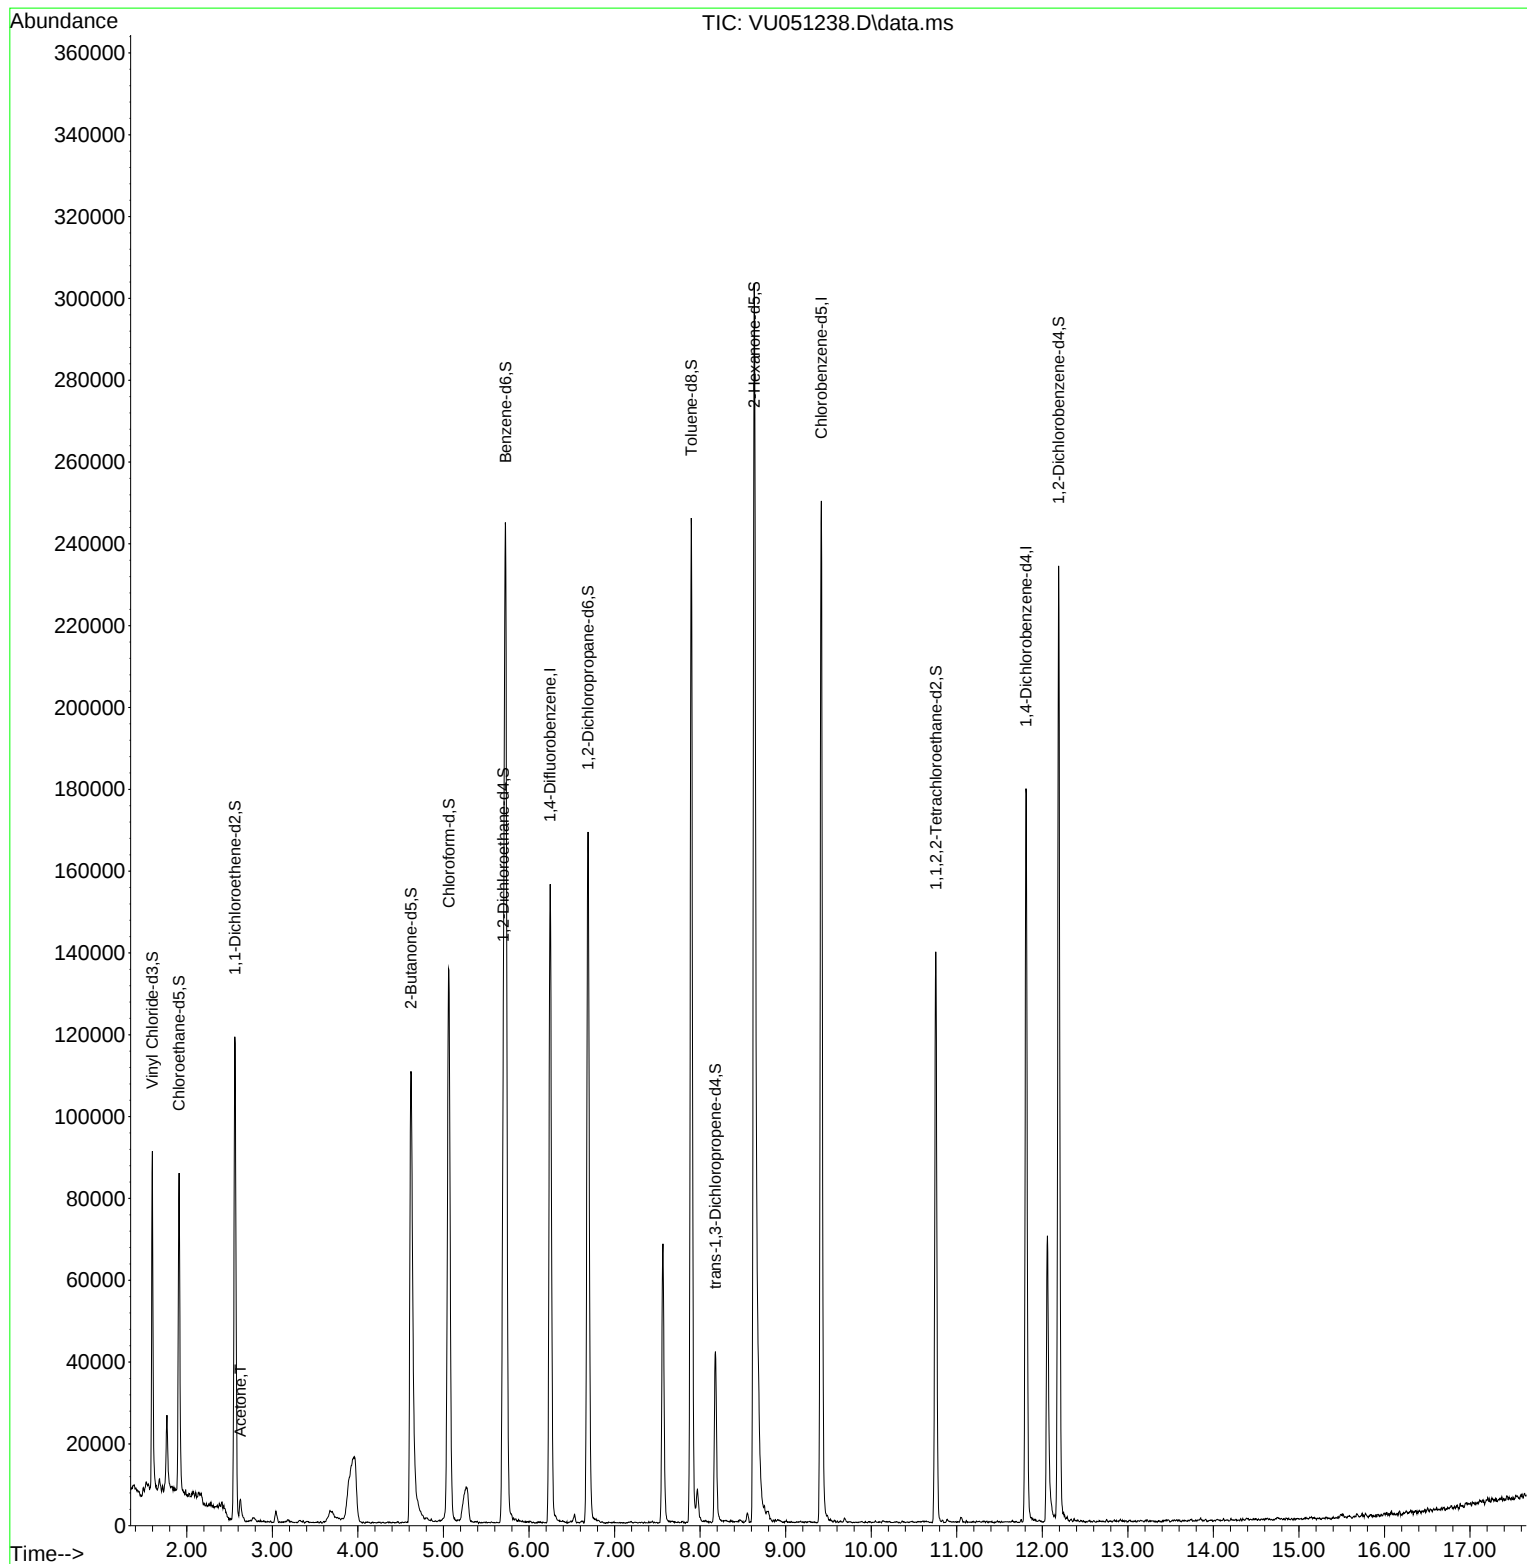

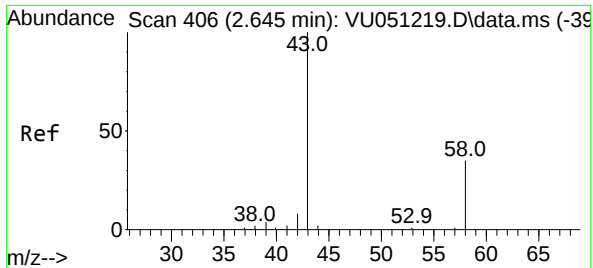

#13
 Acetone
 Concen: 3.727 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. -0.019 min
 Lab File: VU051238.D
 Acq: 07 Oct 2022 23:31

Instrument :
 MSVOA_U
 ClientSampleId :
 EXFS8

Tgt Ion: 43 Resp: 6167
 Ion Ratio Lower Upper
 43 100
 58 33.7 0.0 68.8

