

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051245.D
 Acq On : 08 Oct 2022 02:49
 Operator : JC/MD
 Sample : N4900-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXFT1

Quant Time: Oct 08 23:47:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 08 05:40:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	134595	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	155236	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	52885	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	56629	5.216	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.400%
7) Chloroethane-d5	1.909	69	56055	6.009	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	120.200%
11) 1,1-Dichloroethene-d2	2.565	65	23182	5.401	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	108.000%
20) 2-Butanone-d5	4.620	46	162862	68.133	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	136.260%#
24) Chloroform-d	5.063	84	128897	6.368	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	127.400%#
26) 1,2-Dichloroethane-d4	5.700	65	69916	6.698	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	134.000%#
32) Benzene-d6	5.726	84	227634	5.330	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.600%
36) 1,2-Dichloropropane-d6	6.690	67	84262	5.810	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	116.200%
41) Toluene-d8	7.896	98	174281	4.561	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.200%
43) trans-1,3-Dichloroprop...	8.179	79	23915	5.019	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.400%
46) 2-Hexanone-d5	8.632	63	83062	51.722	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.440%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	72696	6.275	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	125.400%#
66) 1,2-Dichlorobenzene-d4	12.192	152	61303	6.669	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	133.400%#
Target Compounds					Qvalue	
13) Acetone	2.623	43	4647	2.592	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051245.D
Acq On : 08 Oct 2022 02:49
Operator : JC/MD
Sample : N4900-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXFT1

Quant Time: Oct 08 23:47:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 08 05:40:36 2022
Response via : Initial Calibration

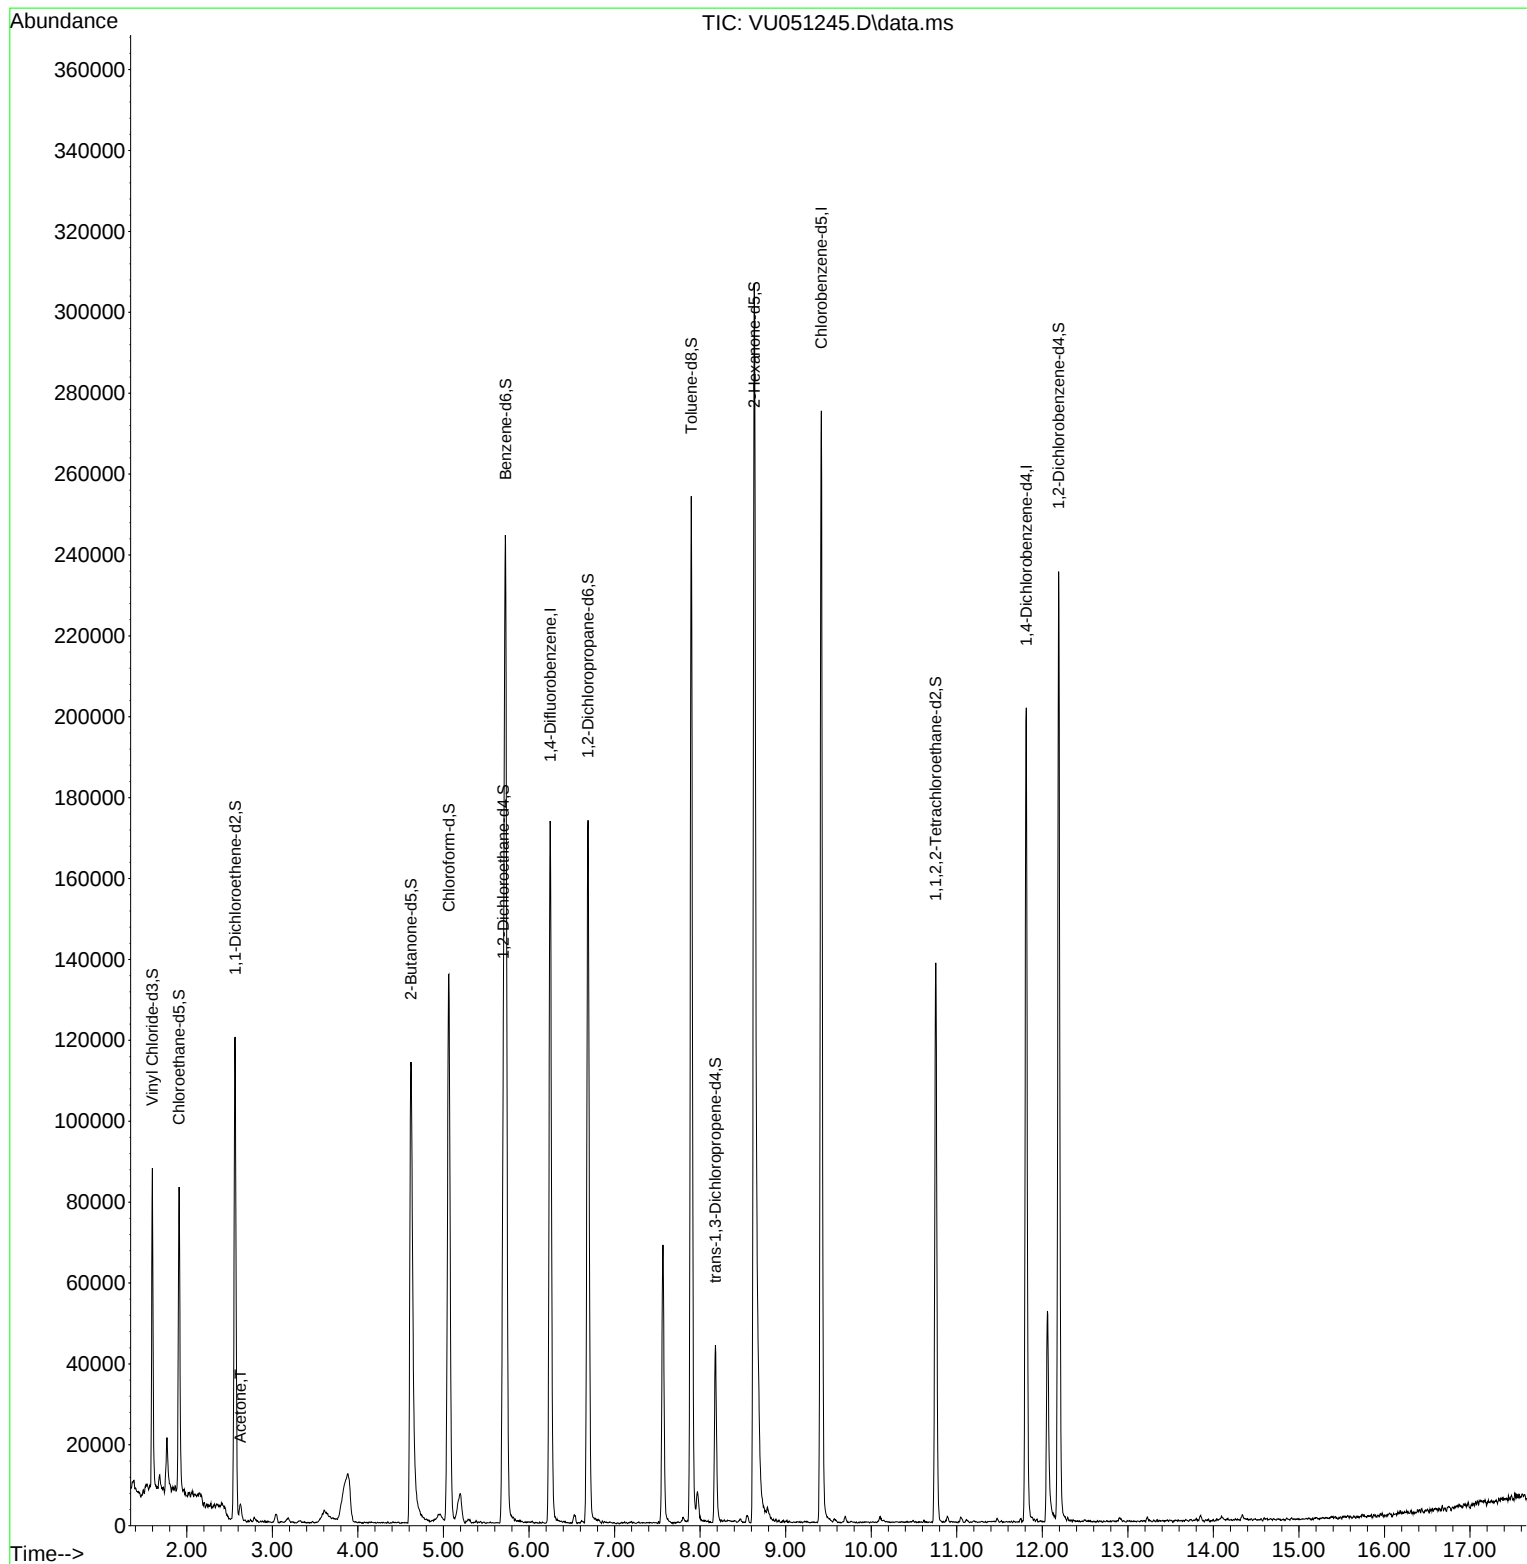

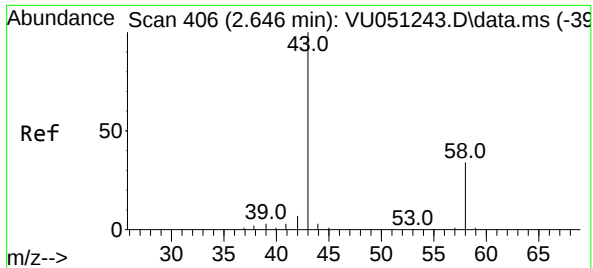

#13
 Acetone
 Concen: 2.592 ug/L
 RT: 2.623 min Scan# 31
 Delta R.T. -0.023 min
 Lab File: VU051245.D
 Acq: 08 Oct 2022 02:49

Instrument :
 MSVOA_U
 ClientSampleId :
 EXFT1

Tgt Ion: 43 Resp: 4647
 Ion Ratio Lower Upper
 43 100
 58 31.4 0.0 68.8

