

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051255.D
 Acq On : 08 Oct 2022 06:56
 Operator : JC/MD
 Sample : N4899-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5H62

Quant Time: Oct 08 23:48:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 08 05:40:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	155297	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	180456	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	59623	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	56516	4.512	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.200%
7) Chloroethane-d5	1.909	69	53847	5.003	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.000%
11) 1,1-Dichloroethene-d2	2.562	65	21910	4.425	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.400%
20) 2-Butanone-d5	4.620	46	154227	55.920	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.840%
24) Chloroform-d	5.060	84	123035	5.268	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.400%
26) 1,2-Dichloroethane-d4	5.700	65	66525	5.523	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.400%
32) Benzene-d6	5.726	84	212443	4.279	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
36) 1,2-Dichloropropane-d6	6.690	67	79824	4.735	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.600%
41) Toluene-d8	7.896	98	160196	3.607	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.200%
43) trans-1,3-Dichloroprop...	8.179	79	23526	4.247	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%
46) 2-Hexanone-d5	8.632	63	80290	43.009	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.020%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	67296	4.997	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.000%
66) 1,2-Dichlorobenzene-d4	12.195	152	53262	5.140	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.800%
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.571	96	3461	0.306	ug/L	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051255.D
Acq On : 08 Oct 2022 06:56
Operator : JC/MD
Sample : N4899-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H62

Quant Time: Oct 08 23:48:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 08 05:40:36 2022
Response via : Initial Calibration

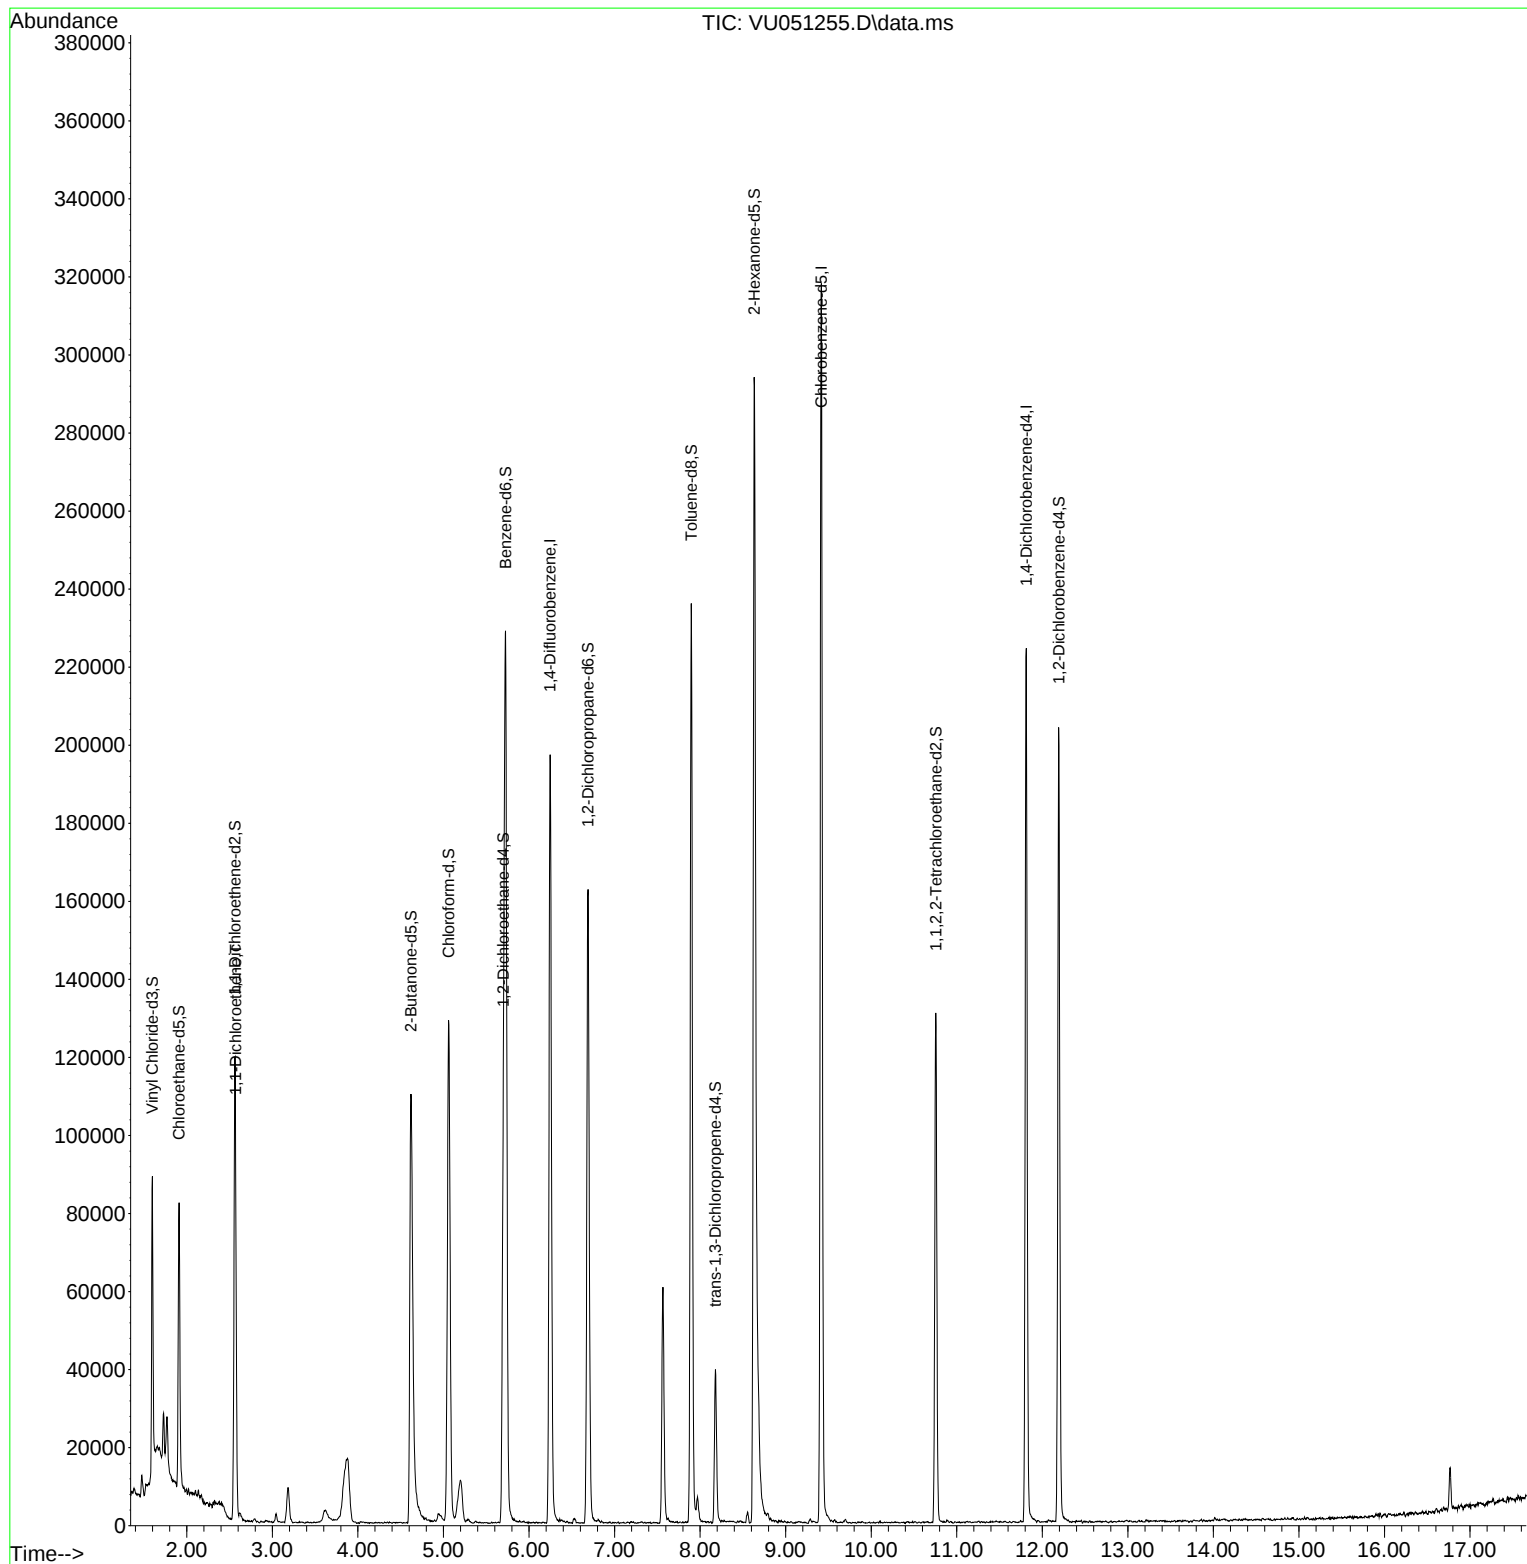

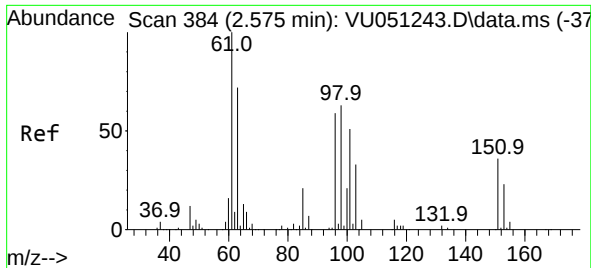

#12
 1,1-Dichloroethene
 Concen: 0.306 ug/L
 RT: 2.571 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VU051255.D
 Acq: 08 Oct 2022 06:56

Instrument :
 MSVOA_U
 ClientSampleId :
 F5H62

Tgt Ion: 96 Resp: 3461
 Ion Ratio Lower Upper
 96 100
 61 321.6 117.6 218.4#
 63 1562.4 85.2 158.2#

