

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051267.D
 Acq On : 08 Oct 2022 11:53
 Operator : JC/MD
 Sample : N4931-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5H83

Quant Time: Oct 08 23:49:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 08 05:40:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	159076	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	188806	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	73934	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	56601	4.411	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.200%
7) Chloroethane-d5	1.909	69	56339	5.110	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.200%
11) 1,1-Dichloroethene-d2	2.562	65	23749	4.682	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	93.600%
20) 2-Butanone-d5	4.620	46	139160	49.258	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.520%
24) Chloroform-d	5.060	84	127793	5.342	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.800%
26) 1,2-Dichloroethane-d4	5.700	65	67784	5.494	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.800%
32) Benzene-d6	5.726	84	222802	4.290	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.800%
36) 1,2-Dichloropropane-d6	6.690	67	82403	4.671	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.400%
41) Toluene-d8	7.896	98	165040	3.552	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.000%
43) trans-1,3-Dichloroprop...	8.179	79	21516	3.713	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.200%
46) 2-Hexanone-d5	8.632	63	68143	34.888	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	69.780%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	63017	4.472	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.400%
66) 1,2-Dichlorobenzene-d4	12.192	152	66166	5.149	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.000%
Target Compounds						
13) Acetone	2.626	43	10357	4.888	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051267.D
Acq On : 08 Oct 2022 11:53
Operator : JC/MD
Sample : N4931-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H83

Quant Time: Oct 08 23:49:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 08 05:40:36 2022
Response via : Initial Calibration

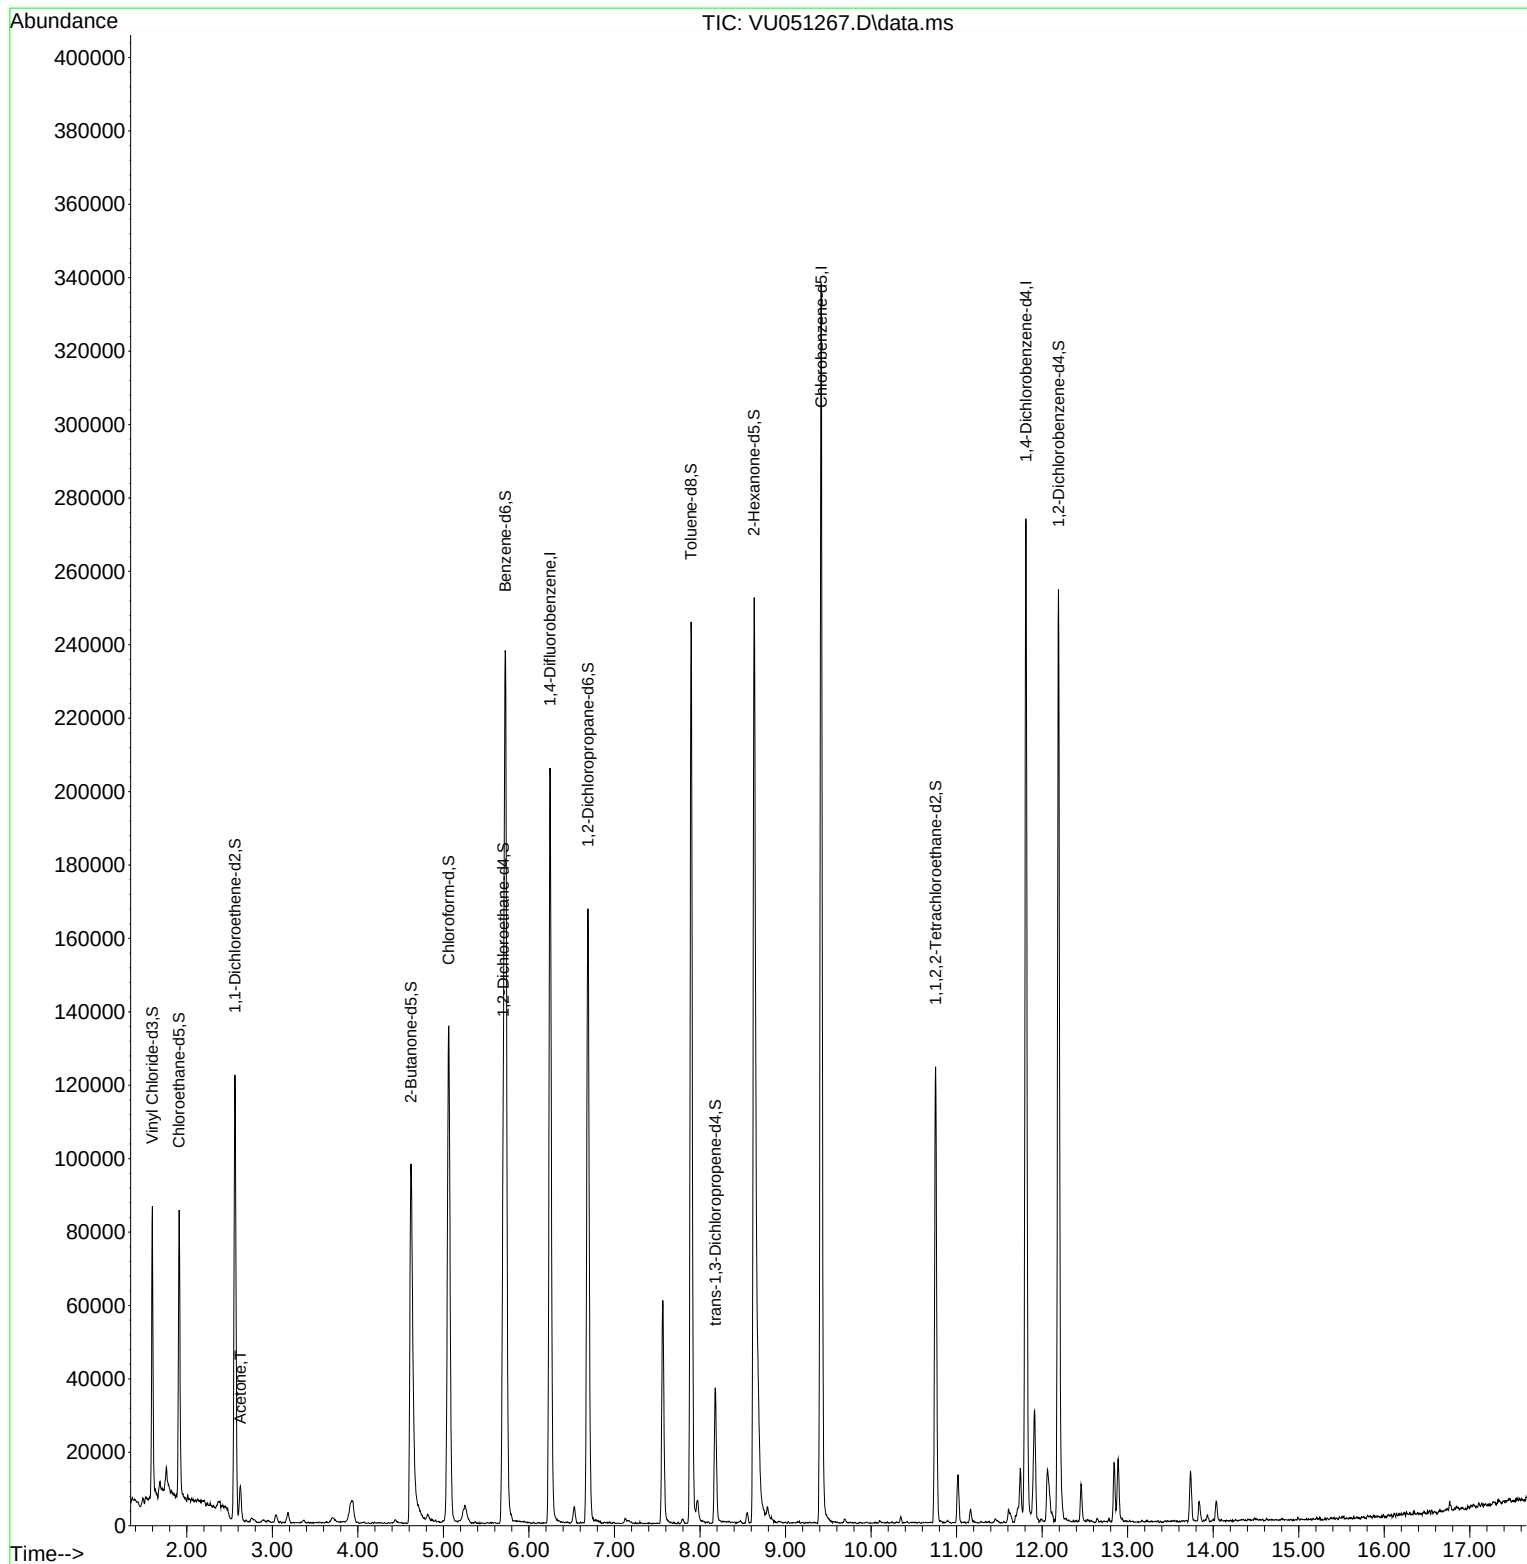

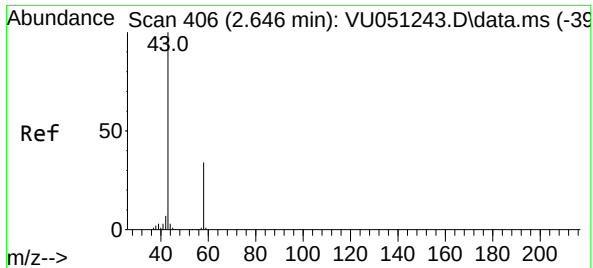

#13
 Acetone
 Concen: 4.888 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. -0.020 min
 Lab File: VU051267.D
 Acq: 08 Oct 2022 11:53

Instrument : MSVOA_U
 ClientSampleId : F5H83

Tgt Ion: 43	Resp: 10357
Ion Ratio	Lower Upper
43	100
58	35.7 0.0 68.8

