

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU100722\  
 Data File : VU051274.D  
 Acq On : 08 Oct 2022 16:05  
 Operator : JC/MD  
 Sample : N4922-03  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 63 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 CB8R3

Quant Time: Oct 08 23:50:40 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR100722WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Oct 08 05:40:36 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|
| -----                         |        |       |          |          |        |          |
| Internal Standards            |        |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 6.247  | 114   | 167618   | 5.000    | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 9.417  | 117   | 191506   | 5.000    | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.812 | 152   | 70249    | 5.000    | ug/L   | 0.00     |
|                               |        |       |          |          |        |          |
| System Monitoring Compounds   |        |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.597  | 65    | 64170    | 4.746    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 95.000%  |
| 7) Chloroethane-d5            | 1.912  | 69    | 60439    | 5.202    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 104.000% |
| 11) 1,1-Dichloroethene-d2     | 2.565  | 65    | 24826    | 4.645    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 92.800%  |
| 20) 2-Butanone-d5             | 4.620  | 46    | 156744   | 52.655   | ug/L   | -0.02    |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 105.300% |
| 24) Chloroform-d              | 5.063  | 84    | 140760   | 5.584    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 111.600% |
| 26) 1,2-Dichloroethane-d4     | 5.700  | 65    | 74268    | 5.713    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 114.200% |
| 32) Benzene-d6                | 5.726  | 84    | 247831   | 4.704    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 94.000%  |
| 36) 1,2-Dichloropropane-d6    | 6.690  | 67    | 91716    | 5.126    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 102.600% |
| 41) Toluene-d8                | 7.896  | 98    | 187780   | 3.984    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 79.600%  |
| 43) trans-1,3-Dichloroprop... | 8.179  | 79    | 23651    | 4.023    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 80.400%  |
| 46) 2-Hexanone-d5             | 8.632  | 63    | 78646    | 39.697   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 79.400%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.754 | 84    | 72873    | 5.099    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 102.000% |
| 66) 1,2-Dichlorobenzene-d4    | 12.192 | 152   | 70385    | 5.765    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 115.200% |
|                               |        |       |          |          |        |          |
| Target Compounds              |        |       |          |          | Qvalue |          |
| 13) Acetone                   | 2.626  | 43    | 11600    | 5.196    | ug/L   | 97       |
| -----                         |        |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU100722\  
Data File : VU051274.D  
Acq On : 08 Oct 2022 16:05  
Operator : JC/MD  
Sample : N4922-03  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 63 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
CB8R3

Quant Time: Oct 08 23:50:40 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR100722WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Oct 08 05:40:36 2022  
Response via : Initial Calibration

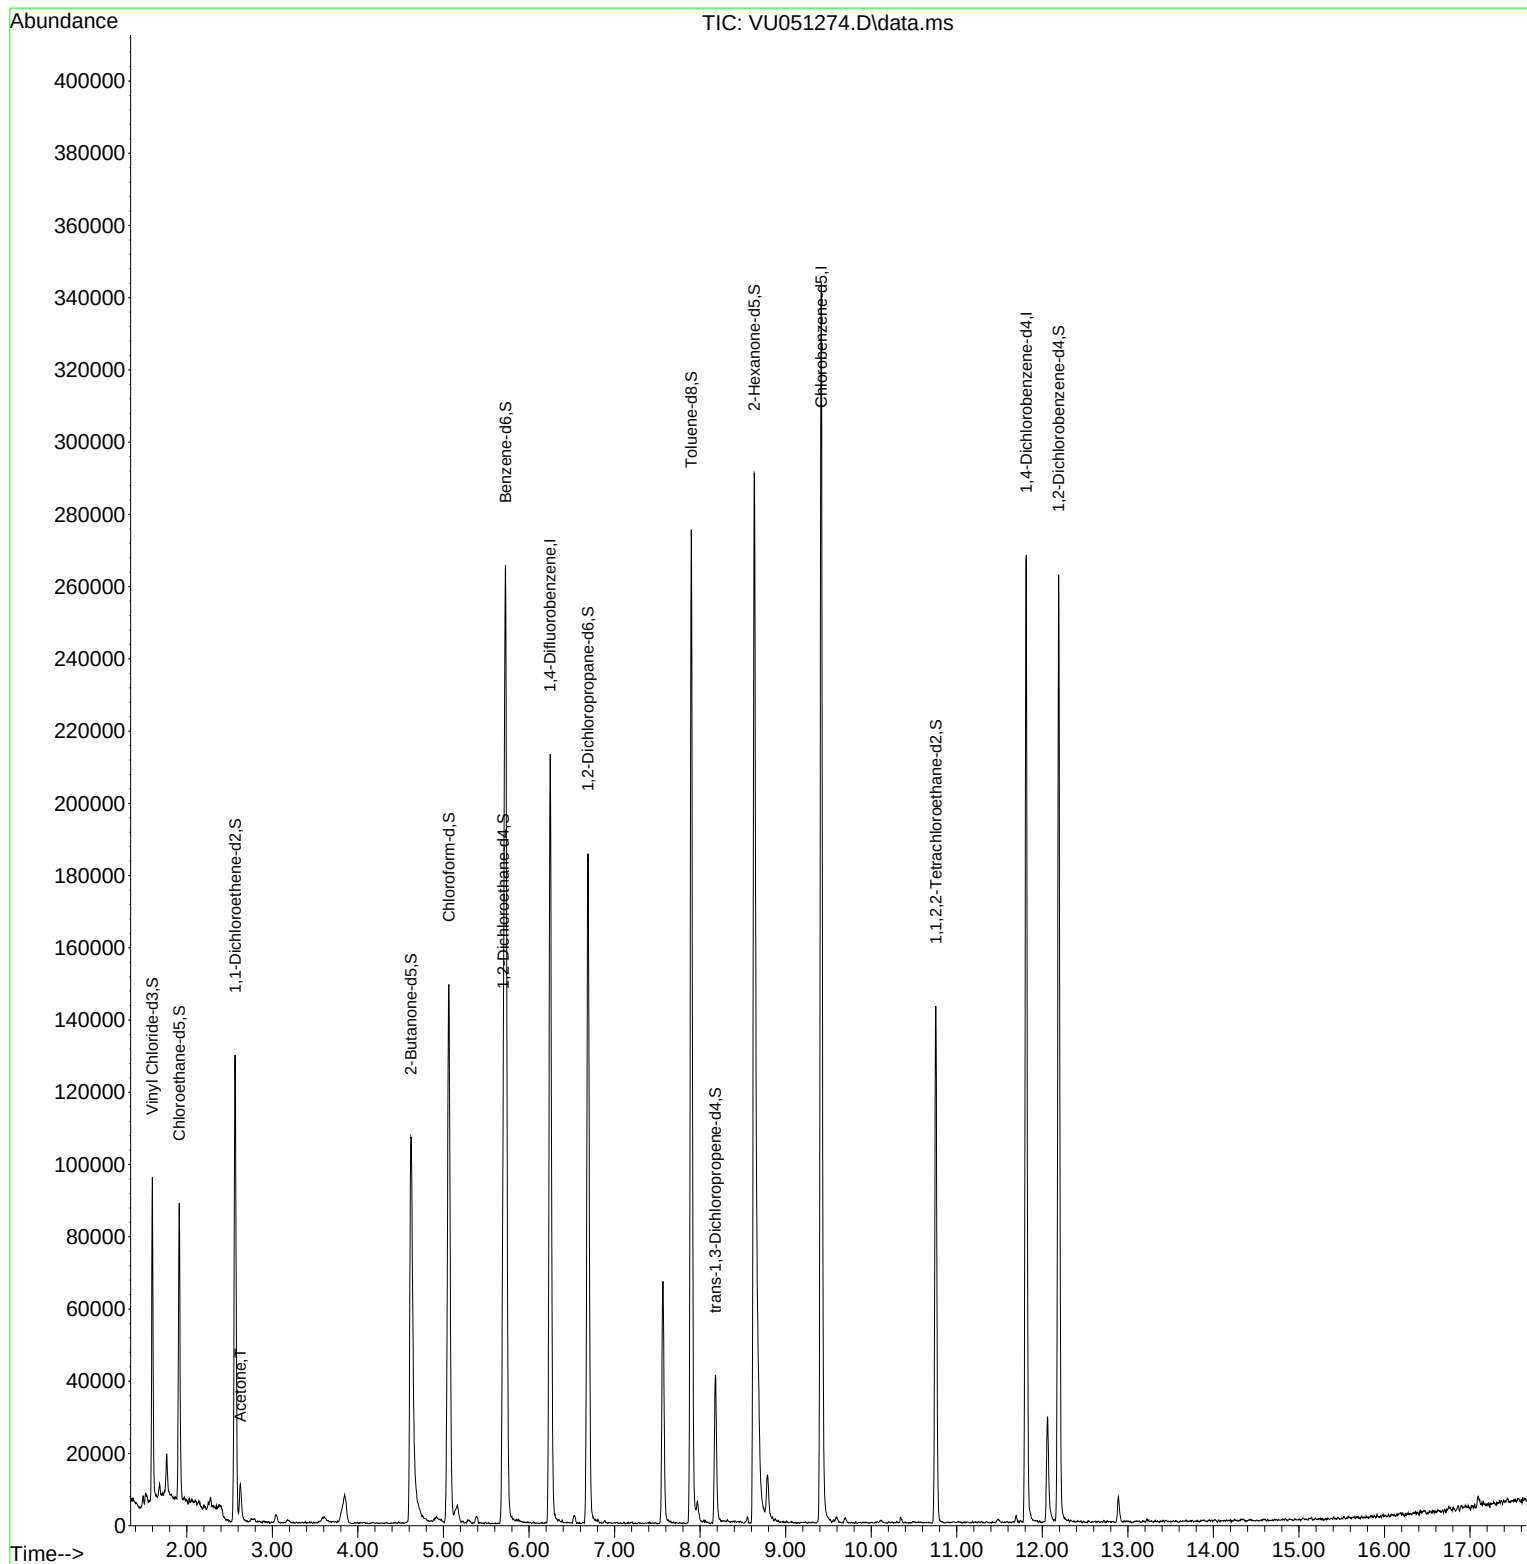

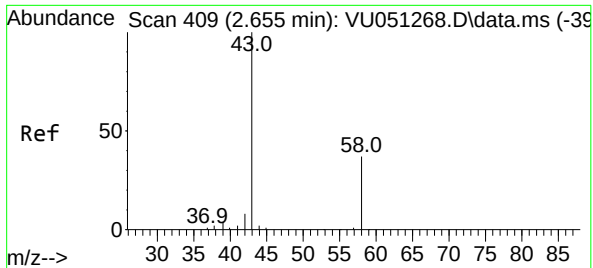

#13  
 Acetone  
 Concen: 5.196 ug/L  
 RT: 2.626 min Scan# 40  
 Delta R.T. -0.019 min  
 Lab File: VU051274.D  
 Acq: 08 Oct 2022 16:05

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 CB8R3

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 43    | Resp: | 11600 |
| Ion Ratio | Lower | Upper |       |
| 43        | 100   |       |       |
| 58        | 36.2  | 0.0   | 68.8  |

