

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051276.D
 Acq On : 08 Oct 2022 16:55
 Operator : JC/MD
 Sample : N4922-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CB8S5

Quant Time: Oct 09 12:23:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 08 05:40:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	169887	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	195878	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	72861	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.598	65	60820	4.438	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.800%
7) Chloroethane-d5	1.913	69	58841	4.997	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.000%
11) 1,1-Dichloroethene-d2	2.565	65	23711	4.377	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.600%
20) 2-Butanone-d5	4.623	46	152783	50.639	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.280%
24) Chloroform-d	5.061	84	135581	5.307	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.200%
26) 1,2-Dichloroethane-d4	5.700	65	72888	5.532	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.600%
32) Benzene-d6	5.726	84	240141	4.457	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.200%
36) 1,2-Dichloropropane-d6	6.687	67	87049	4.757	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.200%
41) Toluene-d8	7.896	98	182442	3.784	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.600%
43) trans-1,3-Dichloroprop...	8.179	79	24121	4.012	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.200%
46) 2-Hexanone-d5	8.633	63	76094	37.552	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.100%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	70998	4.857	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	65735	5.191	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.800%
Target Compounds					Qvalue	
13) Acetone	2.627	43	12679	5.603	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051276.D
Acq On : 08 Oct 2022 16:55
Operator : JC/MD
Sample : N4922-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CB8S5

Quant Time: Oct 09 12:23:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 08 05:40:36 2022
Response via : Initial Calibration

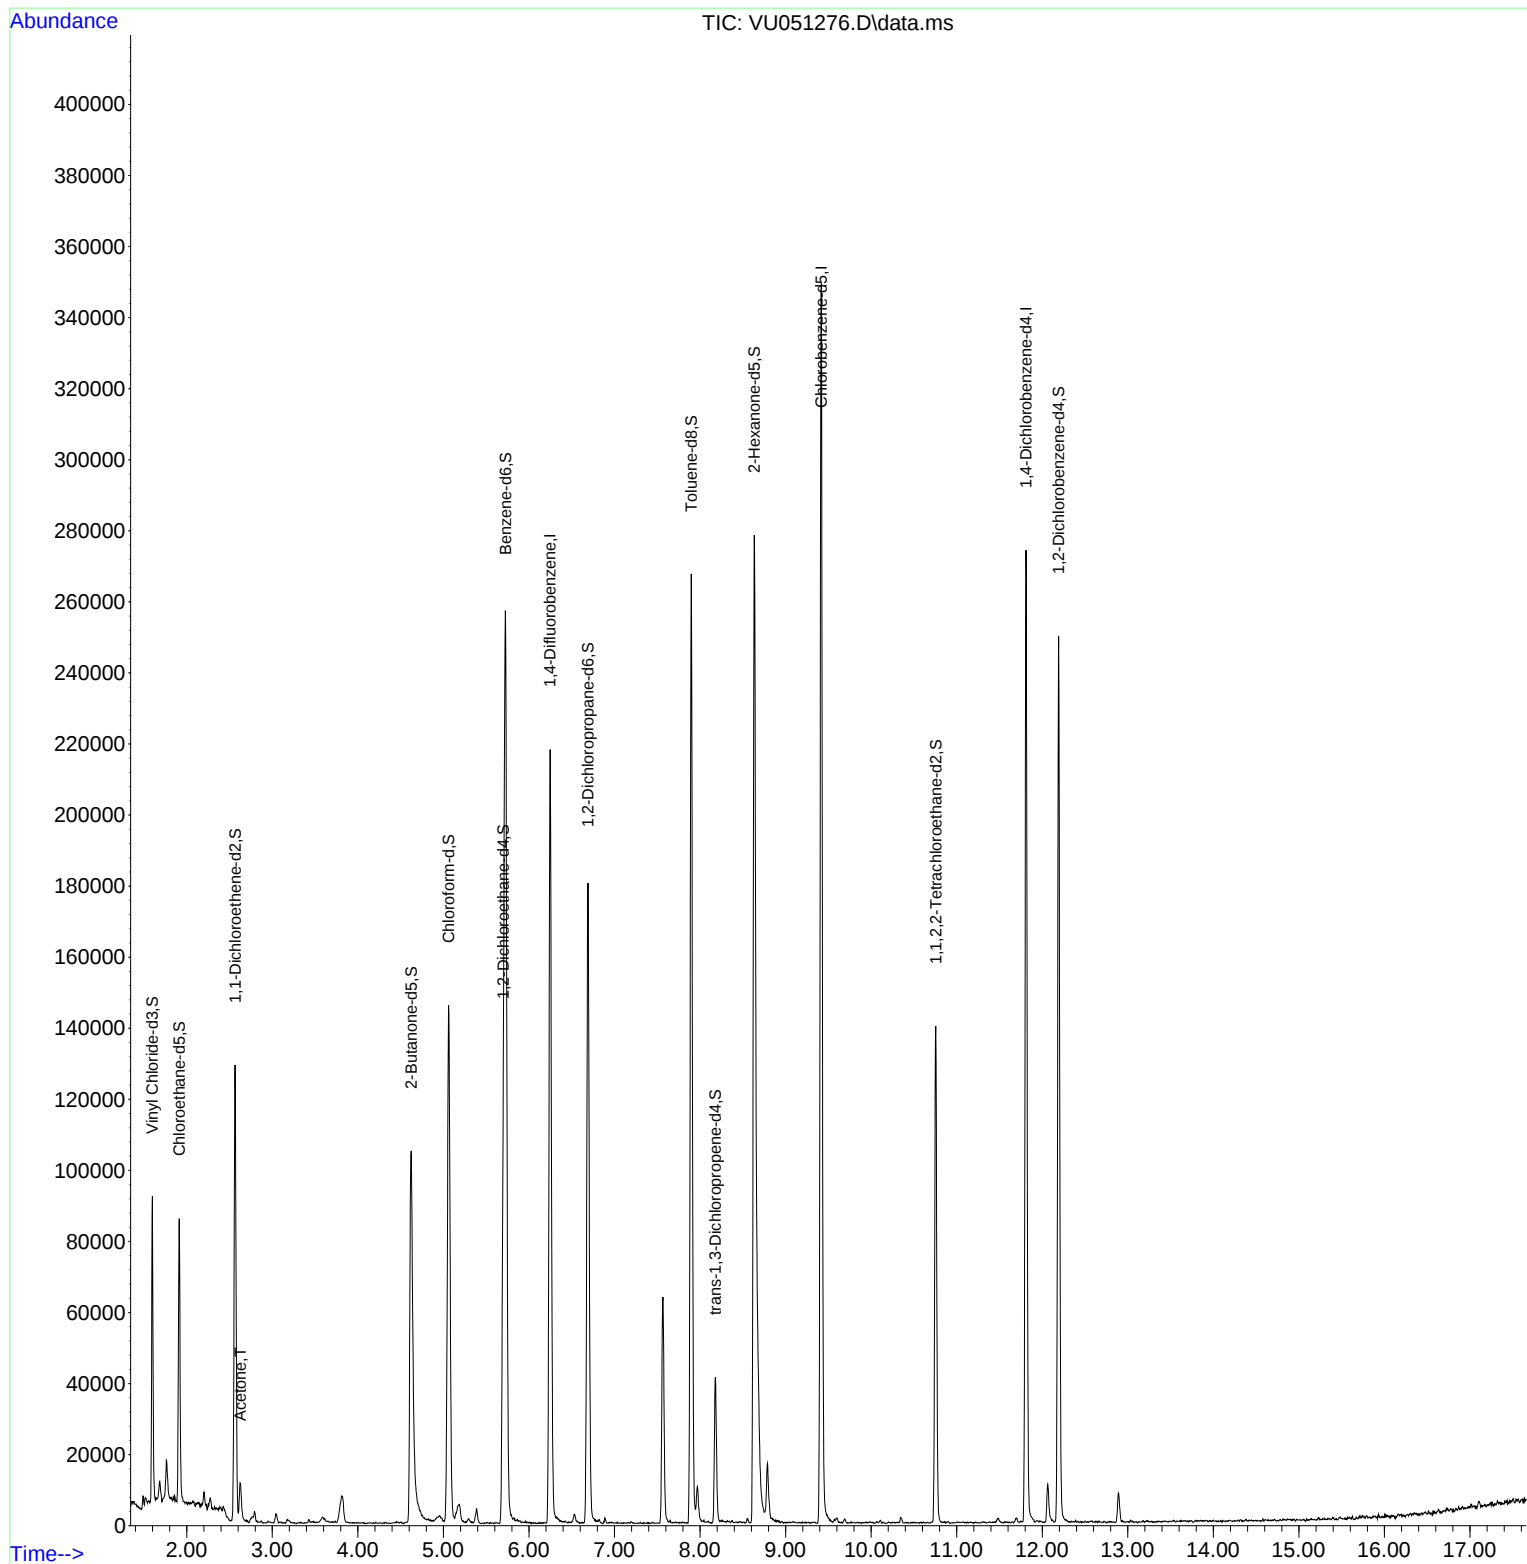

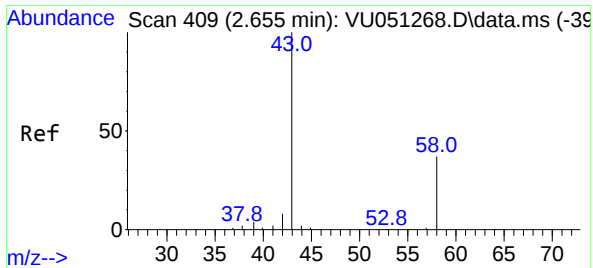

#13
 Acetone
 Concen: 5.603 ug/L
 RT: 2.627 min Scan# 40
 Delta R.T. -0.019 min
 Lab File: VU051276.D
 Acq: 08 Oct 2022 16:55

Instrument :
 MSVOA_U
 ClientSampleId :
 CB8S5

Tgt Ion: 43 Resp: 12679
 Ion Ratio Lower Upper
 43 100
 58 33.1 0.0 68.8

