

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051281.D
 Acq On : 08 Oct 2022 18:56
 Operator : JC/MD
 Sample : N4922-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CB8R1

Quant Time: Oct 08 23:51:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 08 05:40:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	172331	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	190307	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	71823	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	59413	4.274	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.400%
7) Chloroethane-d5	1.912	69	58102	4.865	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.200%
11) 1,1-Dichloroethene-d2	2.565	65	23798	4.331	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.600%
20) 2-Butanone-d5	4.620	46	155342	50.757	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.520%
24) Chloroform-d	5.060	84	133683	5.158	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.200%
26) 1,2-Dichloroethane-d4	5.700	65	71514	5.351	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.000%
32) Benzene-d6	5.726	84	237967	4.545	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.000%
36) 1,2-Dichloropropane-d6	6.690	67	88168	4.959	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.200%
41) Toluene-d8	7.896	98	178277	3.806	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.200%
43) trans-1,3-Dichloroprop...	8.179	79	22895	3.919	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.400%
46) 2-Hexanone-d5	8.632	63	79986	40.628	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.260%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	72557	5.109	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	64418	5.160	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.200%
Target Compounds						Qvalue
13) Acetone	2.623	43	7297	3.179	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051281.D
Acq On : 08 Oct 2022 18:56
Operator : JC/MD
Sample : N4922-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CB8R1

Quant Time: Oct 08 23:51:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 08 05:40:36 2022
Response via : Initial Calibration

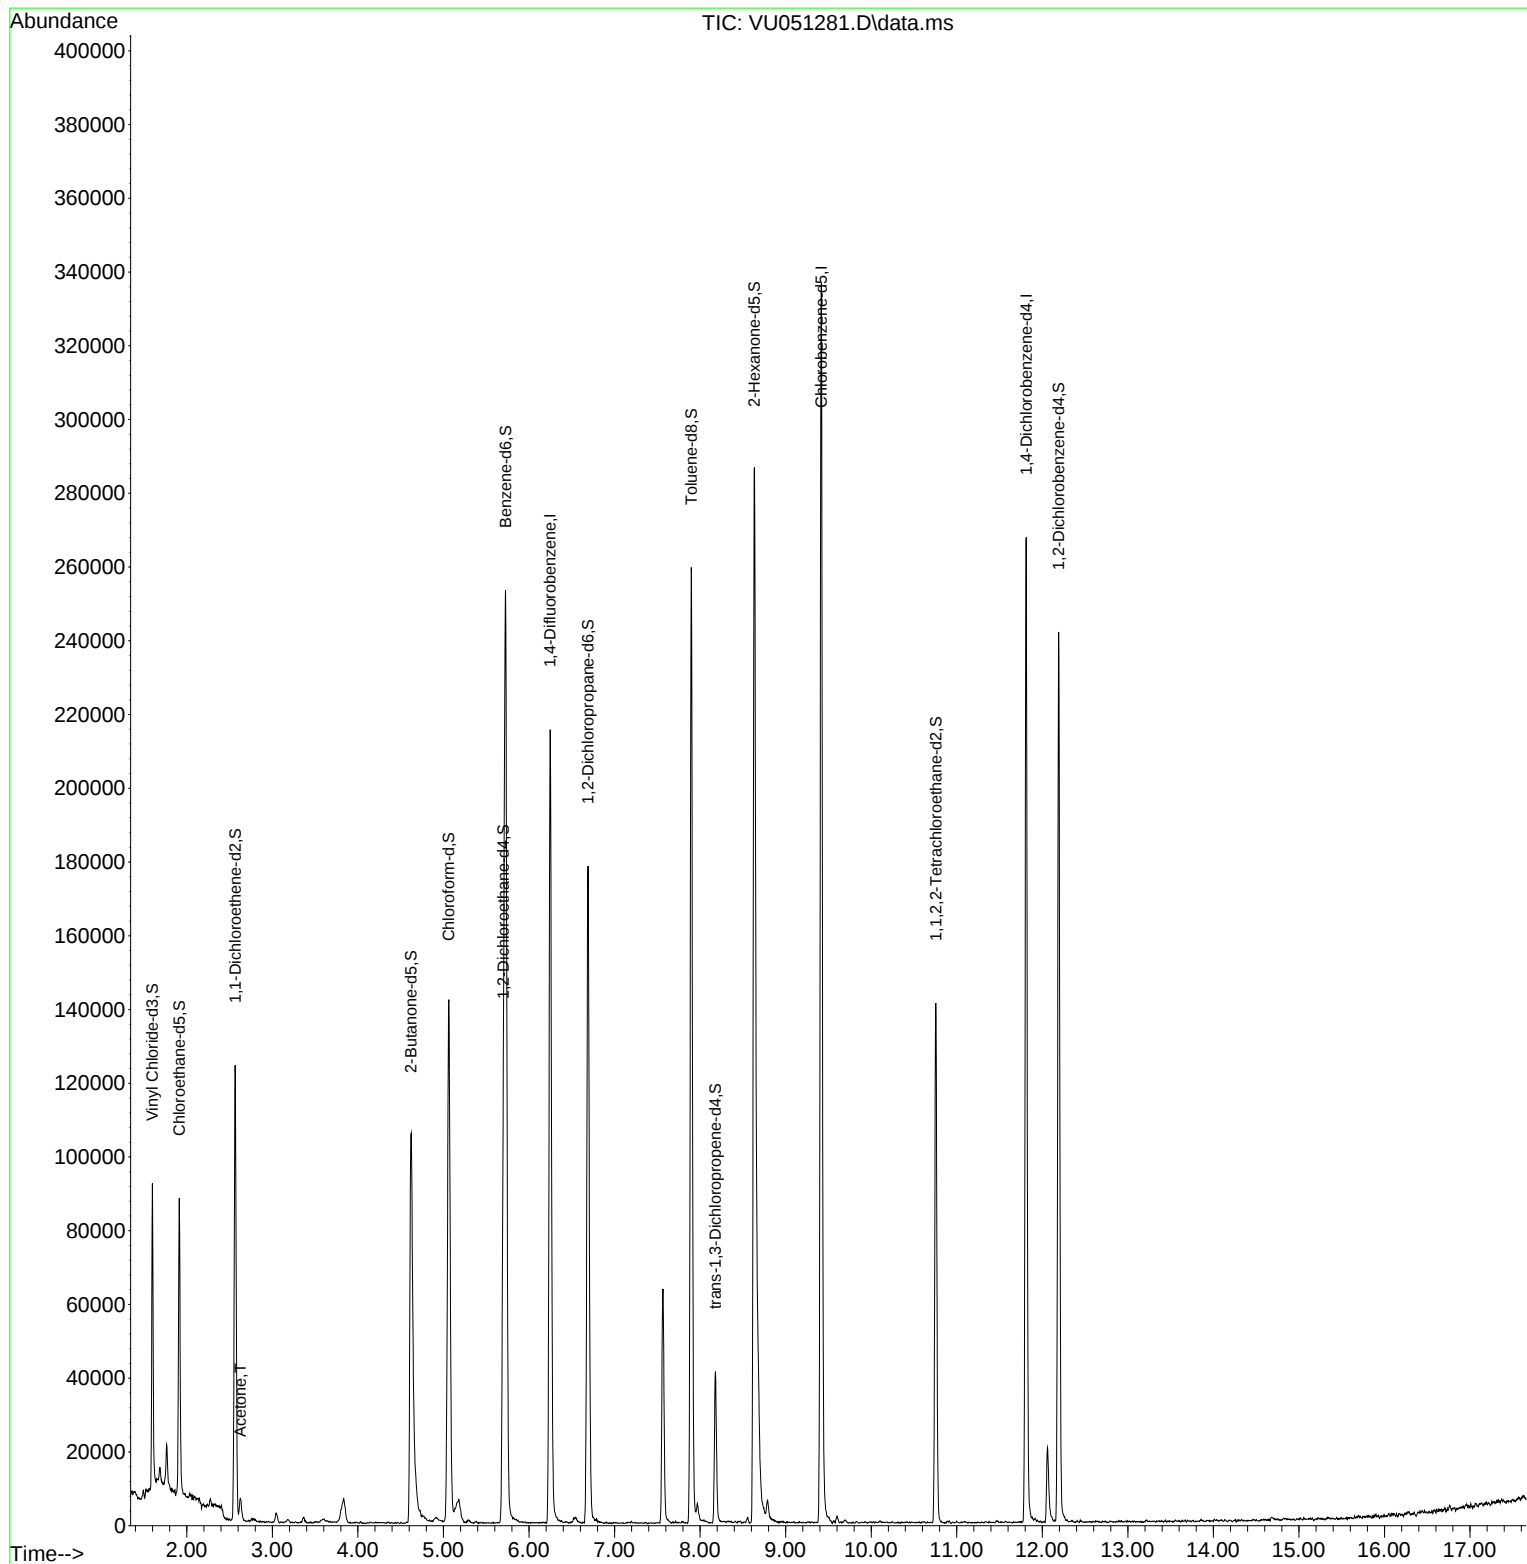

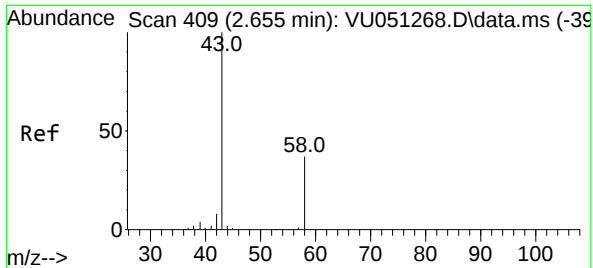

#13
 Acetone
 Concen: 3.179 ug/L
 RT: 2.623 min Scan# 399
 Delta R.T. -0.023 min
 Lab File: VU051281.D
 Acq: 08 Oct 2022 18:56

Instrument :
 MSVOA_U
 ClientSampleId :
 CB8R1

Tgt Ion: 43 Resp: 7297
 Ion Ratio Lower Upper
 43 100
 58 34.7 0.0 68.8

