

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051220.D
 Acq On : 07 Oct 2022 15:56
 Operator : JC/MD
 Sample : VU1007WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK106

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	96	rVB	105829	129410	15.62%	1.994%
2	1.909	169	177	192	rBV	94787	126419	15.26%	1.948%
3	2.562	368	380	396	rBV	165631	273374	33.01%	4.213%
4	3.044	514	530	542	rVB2	16944	31664	3.82%	0.488%
5	4.642	1014	1027	1065	rBV	102864	352845	42.60%	5.438%
6	5.063	1143	1158	1180	rBV	155333	341903	41.28%	5.269%
7	5.176	1185	1193	1203	rVB	4391	9344	1.13%	0.144%
8	5.722	1343	1363	1394	rBV2	301800	795432	96.04%	12.259%
9	6.250	1510	1527	1555	rBV	250093	477741	57.68%	7.363%
10	6.533	1604	1615	1631	rVB10	7351	15692	1.89%	0.242%
11	6.690	1649	1664	1680	rBV	200449	389925	47.08%	6.009%
12	7.565	1921	1936	1959	rBV	83201	156086	18.85%	2.406%
13	7.896	2026	2039	2054	rBV	324082	572203	69.09%	8.819%
14	7.970	2055	2062	2077	rVB	13699	25549	3.08%	0.394%
15	8.179	2117	2127	2150	rBV2	52384	93412	11.28%	1.440%
16	8.552	2235	2243	2252	rBV2	6310	9632	1.16%	0.148%
17	8.639	2256	2270	2307	rBV2	363251	828226	100.00%	12.765%
18	9.417	2497	2512	2538	rBV	370964	628242	75.85%	9.682%
19	9.571	2552	2560	2572	rVB3	6267	8834	1.07%	0.136%
20	9.693	2585	2598	2610	rBV3	5933	9680	1.17%	0.149%
21	10.111	2717	2728	2738	rBV5	6546	13826	1.67%	0.213%
22	10.754	2911	2928	2945	rBV	148215	245170	29.60%	3.779%
23	11.812	3245	3257	3274	rBV	291450	474650	57.31%	7.315%
24	12.192	3362	3375	3393	rBV	272815	459711	55.51%	7.085%
25	13.844	3882	3889	3902	rBV5	5516	9708	1.17%	0.150%
26	14.333	4033	4041	4051	rBV4	5689	9804	1.18%	0.151%




Sum of corrected areas: 6488482

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051220.D
Acq On : 07 Oct 2022 15:56
Operator : JC/MD
Sample : VU1007WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK106

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

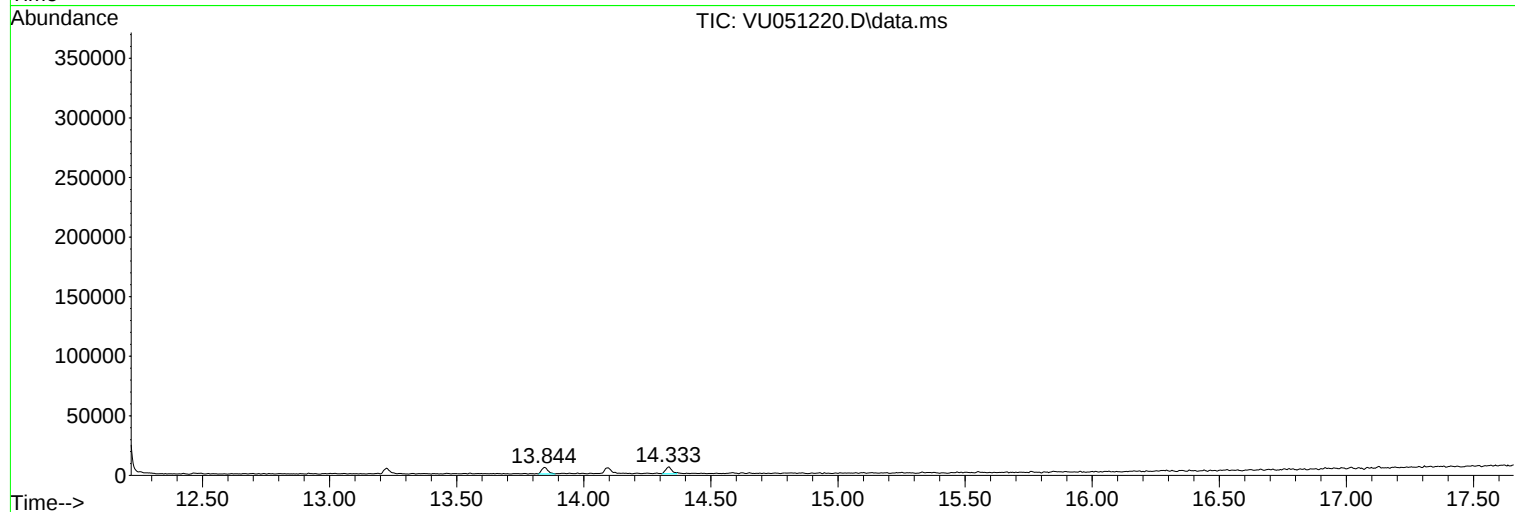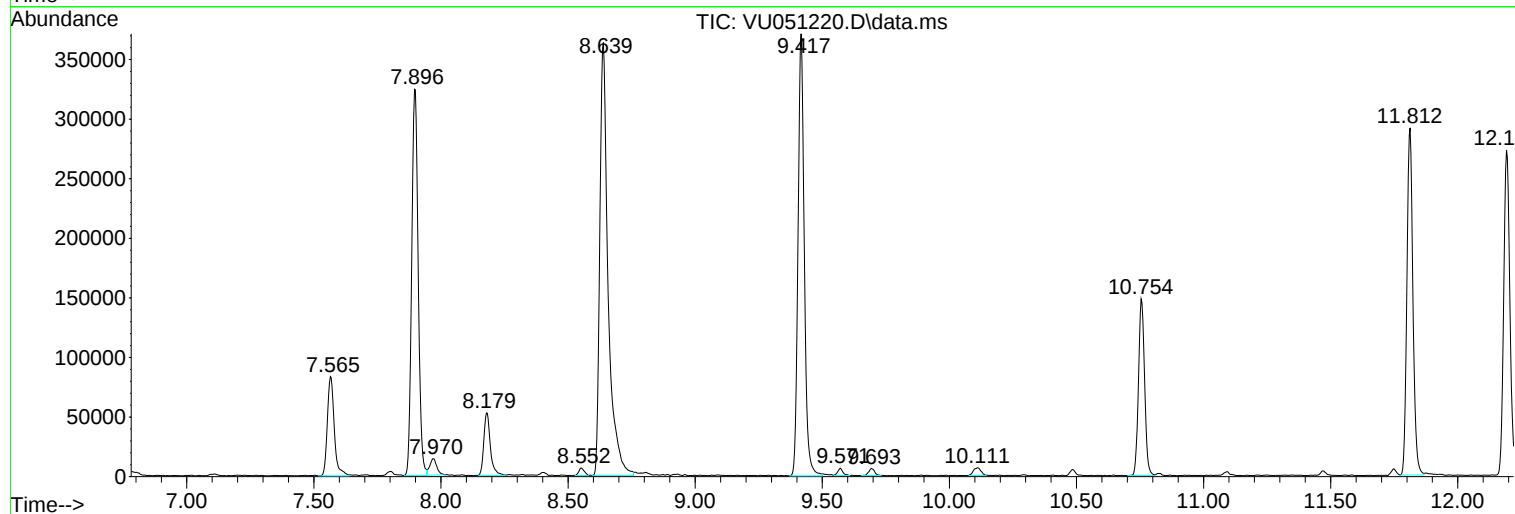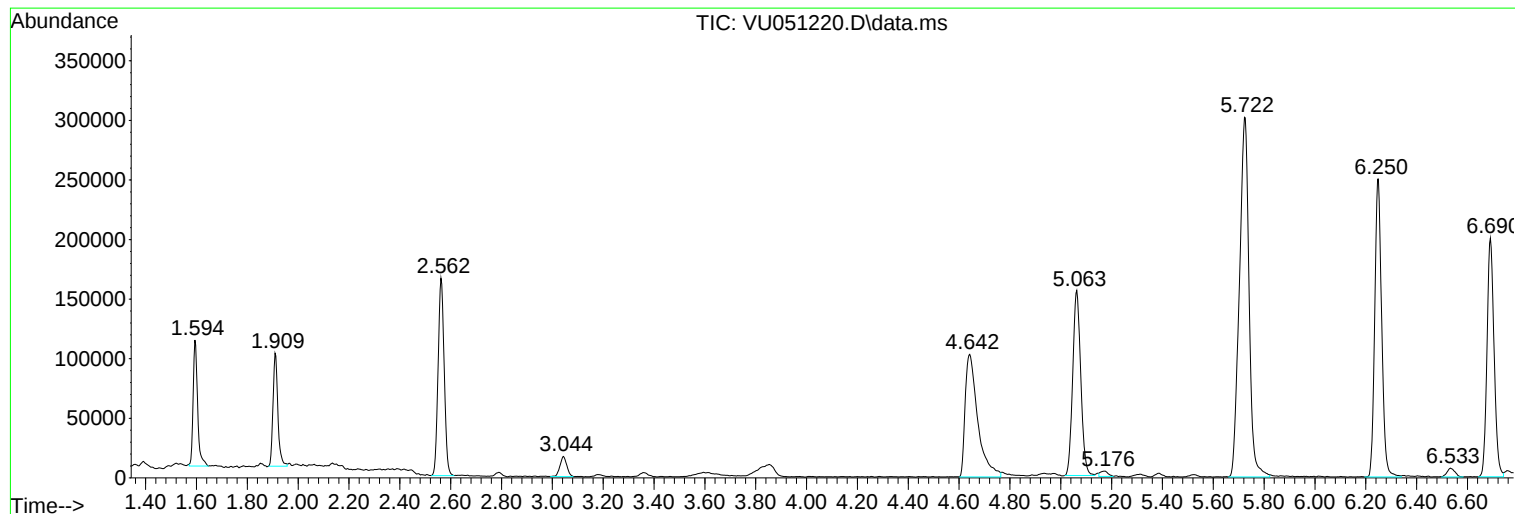

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051220.D
Acq On : 07 Oct 2022 15:56
Operator : JC/MD
Sample : VU1007WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK106

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051220.D
Acq On : 07 Oct 2022 15:56
Operator : JC/MD
Sample : VU1007WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK106

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc