

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051221.D
 Acq On : 07 Oct 2022 16:29
 Operator : JC/MD
 Sample : N4866-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	95	rVB	90672	107661	13.64%	1.813%
2	1.909	169	177	190	rBV	85299	112117	14.21%	1.888%
3	2.562	368	380	400	rVB	142358	233736	29.62%	3.936%
4	3.044	519	530	541	rBV2	14064	25444	3.22%	0.428%
5	3.864	760	785	787	rBV	10467	28009	3.55%	0.472%
6	4.642	1014	1027	1076	rBV	94233	334768	42.42%	5.638%
7	5.063	1143	1158	1180	rVB	146089	320904	40.66%	5.404%
8	5.173	1180	1192	1195	rBV	4852	8348	1.06%	0.141%
9	5.726	1343	1364	1387	rBV2	283158	737966	93.51%	12.428%
10	6.250	1513	1527	1552	rBV	218612	426617	54.06%	7.184%
11	6.529	1605	1614	1627	rVB4	5155	10309	1.31%	0.174%
12	6.690	1650	1664	1683	rBV	190191	372192	47.16%	6.268%
13	7.568	1922	1937	1961	rBV	78411	144389	18.30%	2.432%
14	7.896	2026	2039	2055	rBV	300242	524509	66.46%	8.833%
15	7.973	2055	2063	2080	rVB2	12178	24513	3.11%	0.413%
16	8.182	2117	2128	2149	rBV2	48288	86286	10.93%	1.453%
17	8.639	2257	2270	2311	rBV3	334556	789159	100.00%	13.290%
18	9.417	2498	2512	2538	rBV	334602	570741	72.32%	9.612%
19	10.758	2917	2929	2943	rBV	141792	230110	29.16%	3.875%
20	11.812	3245	3257	3280	rBV2	262120	427601	54.18%	7.201%
21	12.192	3364	3375	3397	rBV	252545	422676	53.56%	7.118%




Sum of corrected areas: 5938055

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051221.D
Acq On : 07 Oct 2022 16:29
Operator : JC/MD
Sample : N4866-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

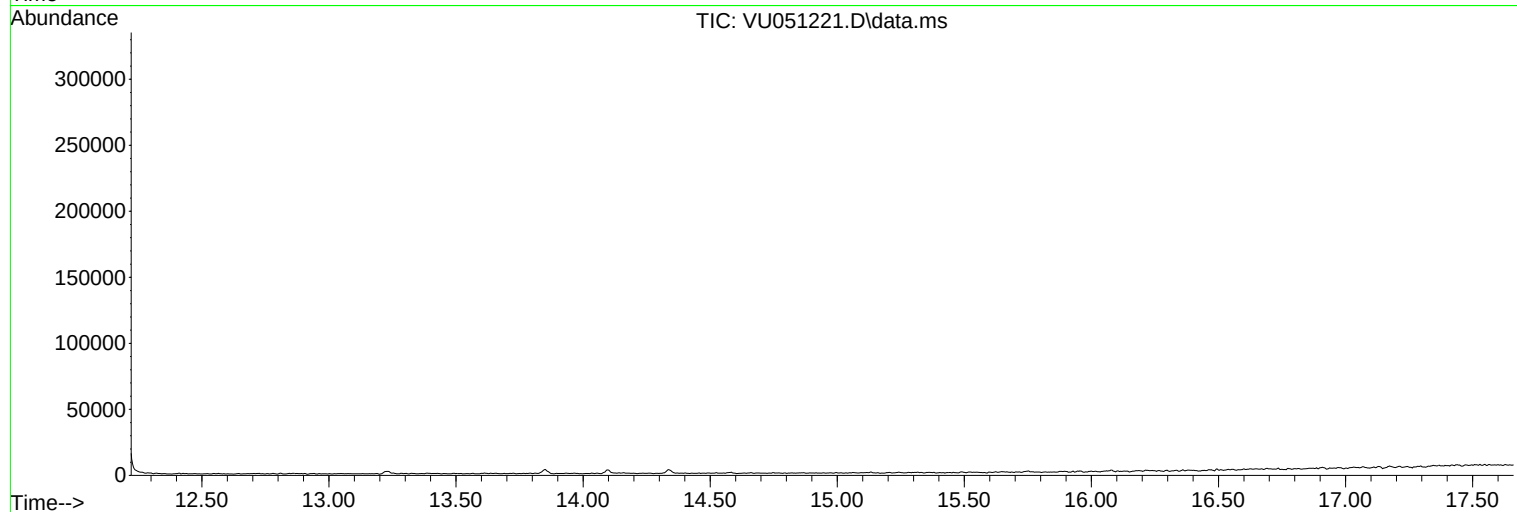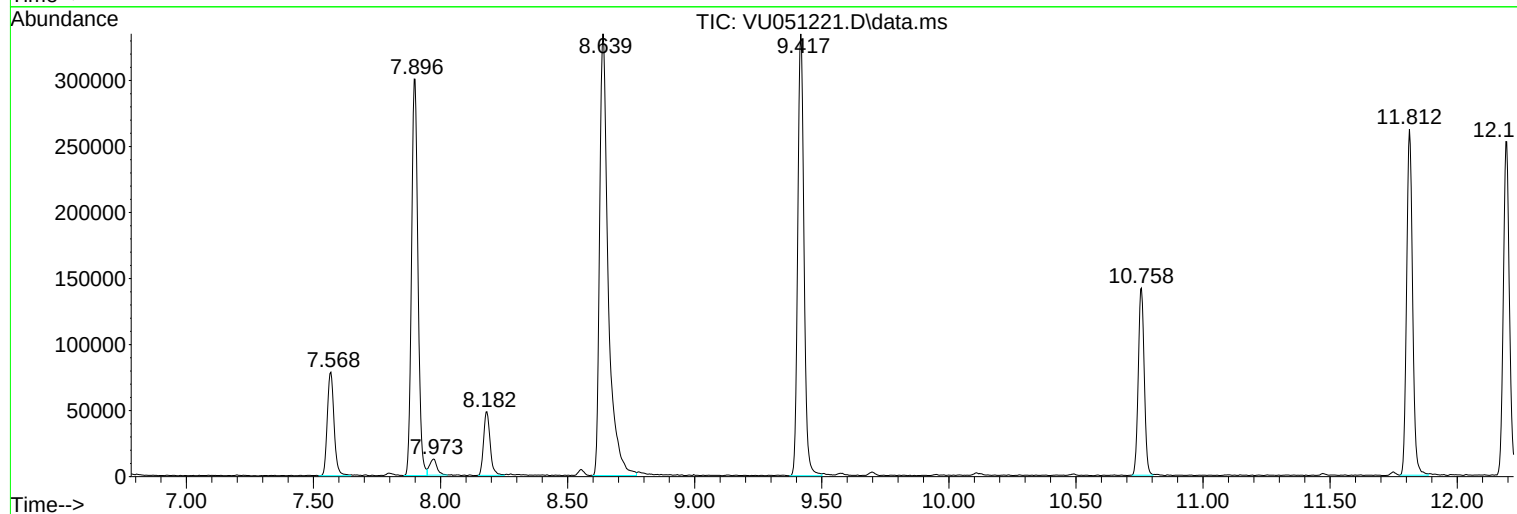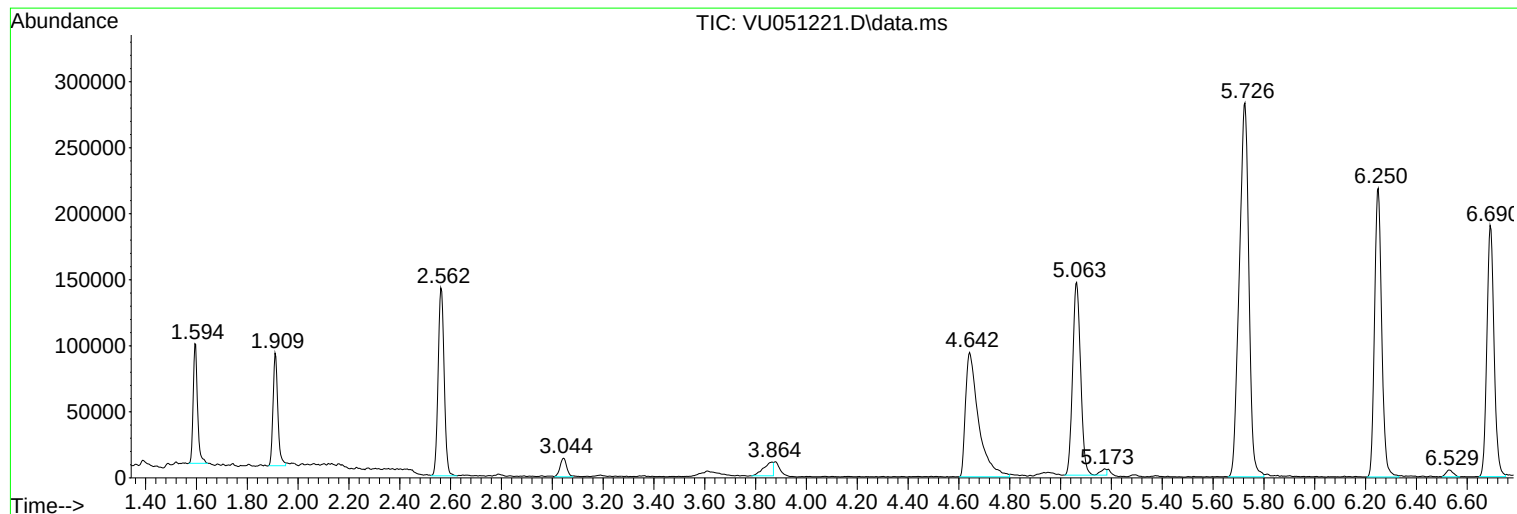

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051221.D
Acq On : 07 Oct 2022 16:29
Operator : JC/MD
Sample : N4866-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051221.D
Acq On : 07 Oct 2022 16:29
Operator : JC/MD
Sample : N4866-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
