

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051222.D
 Acq On : 07 Oct 2022 16:54
 Operator : JC/MD
 Sample : N4873-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ50

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	71	80	92	rBV	93737	108645	14.60%	1.755%
2	1.768	127	133	144	rVB3	19916	25373	3.41%	0.410%
3	1.909	169	177	193	rVB	83256	111403	14.97%	1.800%
4	2.562	368	380	393	rBV	139368	227410	30.56%	3.674%
5	2.629	393	401	422	rVB2	5884	12381	1.66%	0.200%
6	2.758	430	441	460	rBV	17123	33594	4.51%	0.543%
7	3.041	520	529	542	rVB3	4719	8427	1.13%	0.136%
8	3.864	758	785	786	rBV2	11096	34970	4.70%	0.565%
9	4.623	1008	1021	1045	rBV	122204	308629	41.47%	4.987%
10	5.060	1141	1157	1175	rBV	143223	315263	42.36%	5.094%
11	5.208	1181	1203	1220	rVB	9358	33794	4.54%	0.546%
12	5.726	1343	1364	1383	rBV3	276335	718523	96.54%	11.609%
13	6.250	1513	1527	1550	rBV	262026	505959	67.98%	8.175%
14	6.690	1650	1664	1687	rBV	183941	362305	48.68%	5.854%
15	7.565	1924	1936	1955	rBV	78956	140185	18.84%	2.265%
16	7.896	2023	2039	2054	rBV	297328	519039	69.74%	8.386%
17	7.970	2055	2062	2082	rVB2	11956	22854	3.07%	0.369%
18	8.179	2117	2127	2145	rBV2	48442	84005	11.29%	1.357%
19	8.632	2256	2268	2304	rBV4	328212	744261	100.00%	12.025%
20	8.787	2309	2316	2326	rVB6	7569	12224	1.64%	0.198%
21	9.417	2499	2512	2536	rBV	399026	674475	90.62%	10.897%
22	9.571	2550	2560	2576	rVB	5765	9337	1.25%	0.151%
23	9.690	2589	2597	2608	rVB3	5065	8023	1.08%	0.130%
24	10.102	2716	2725	2737	rBV6	4394	8922	1.20%	0.144%
25	10.754	2917	2928	2943	rBV	146702	234057	31.45%	3.782%
26	11.812	3244	3257	3275	rBV	308961	508963	68.39%	8.223%
27	12.192	3362	3375	3397	rBV	251353	416253	55.93%	6.725%




Sum of corrected areas: 6189274

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051222.D
Acq On : 07 Oct 2022 16:54
Operator : JC/MD
Sample : N4873-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

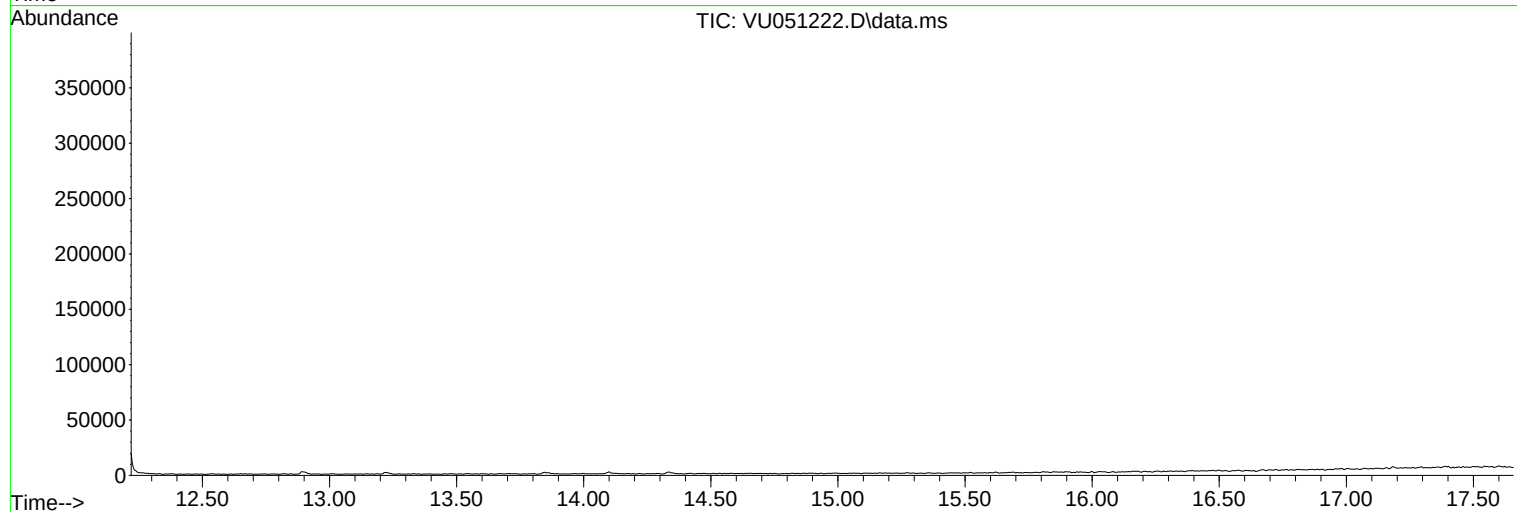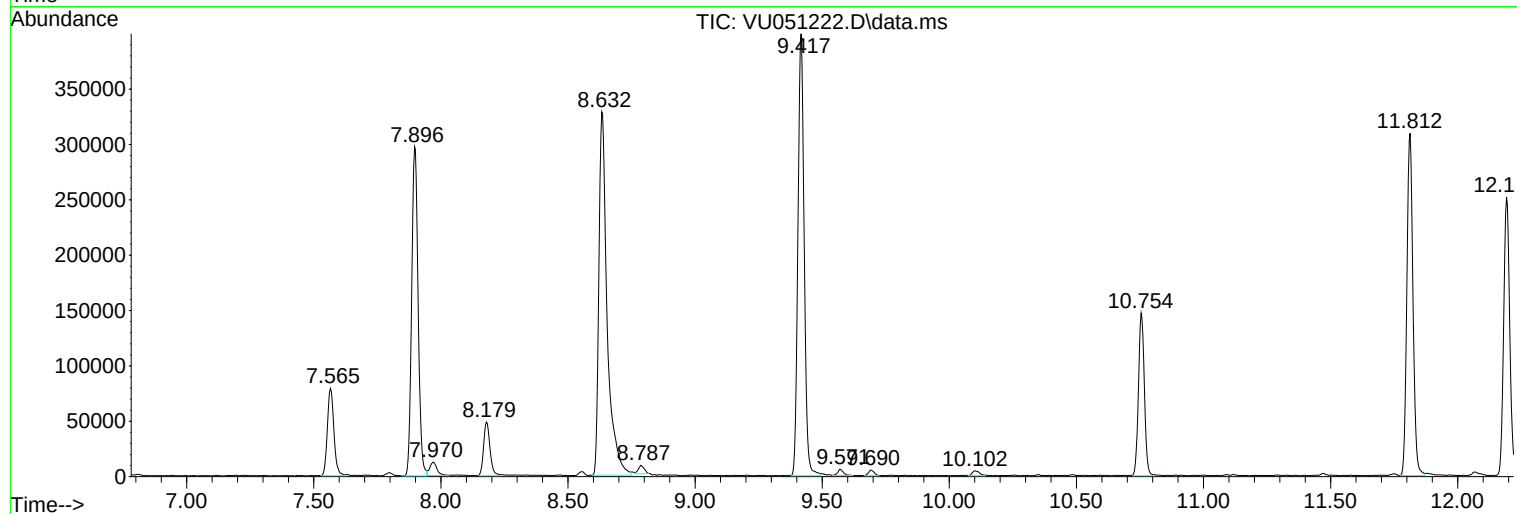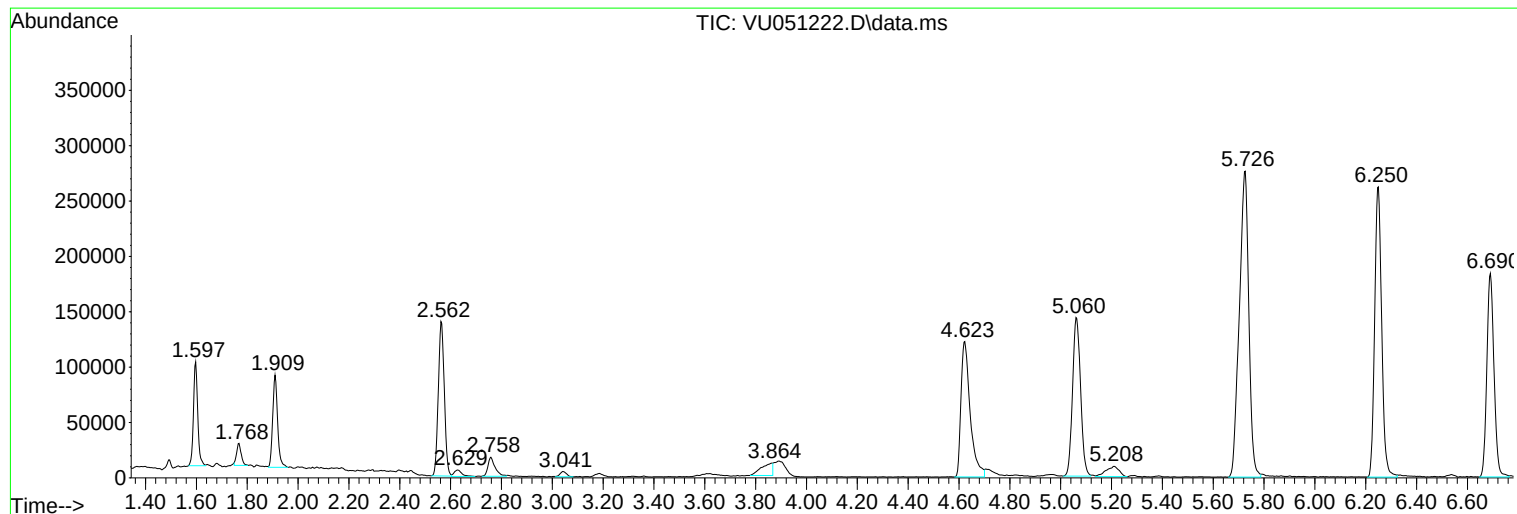

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051222.D
Acq On : 07 Oct 2022 16:54
Operator : JC/MD
Sample : N4873-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051222.D
Acq On : 07 Oct 2022 16:54
Operator : JC/MD
Sample : N4873-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc