

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051231.D
 Acq On : 07 Oct 2022 20:37
 Operator : JC/MD
 Sample : N4872-12DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXFX6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051231.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	71	79	95	rBV	101947	119271	6.40%	1.237%
2	1.909	169	177	189	rBV	94532	122657	6.59%	1.273%
3	2.562	368	380	395	rBV	155725	250886	13.47%	2.603%
4	3.044	517	530	545	rVB2	19902	37945	2.04%	0.394%
5	3.182	558	573	590	rBV	22889	54197	2.91%	0.562%
6	3.848	749	780	781	rBV3	13759	47165	2.53%	0.489%
7	4.639	1008	1026	1064	rBV3	133465	451421	24.24%	4.684%
8	5.060	1141	1157	1178	rBV	152799	338664	18.18%	3.514%
9	5.192	1182	1198	1213	rVB	6661	22736	1.22%	0.236%
10	5.722	1343	1363	1387	rBV2	284161	744411	39.97%	7.723%
11	6.247	1513	1526	1552	rBV	233766	456130	24.49%	4.732%
12	6.690	1648	1664	1681	rBV	192406	377588	20.27%	3.918%
13	7.565	1924	1936	1954	rBV	78430	138326	7.43%	1.435%
14	7.896	2025	2039	2055	rBV	301007	523971	28.13%	5.436%
15	8.179	2117	2127	2142	rBV	47885	82983	4.46%	0.861%
16	8.639	2254	2270	2307	rBV3	344903	780300	41.89%	8.096%
17	9.417	2499	2512	2541	rBV2	369429	858683	46.10%	8.909%
18	10.754	2913	2928	2947	rBV	146865	241460	12.96%	2.505%
19	11.745	3224	3236	3246	rBV	281876	445686	23.93%	4.624%
20	11.835	3246	3264	3292	rVB2	769687	1681291	90.27%	17.444%
21	12.208	3363	3380	3409	rBV3	902614	1862535	100.00%	19.324%




Sum of corrected areas: 9638306

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051231.D
Acq On : 07 Oct 2022 20:37
Operator : JC/MD
Sample : N4872-12DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXFX6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

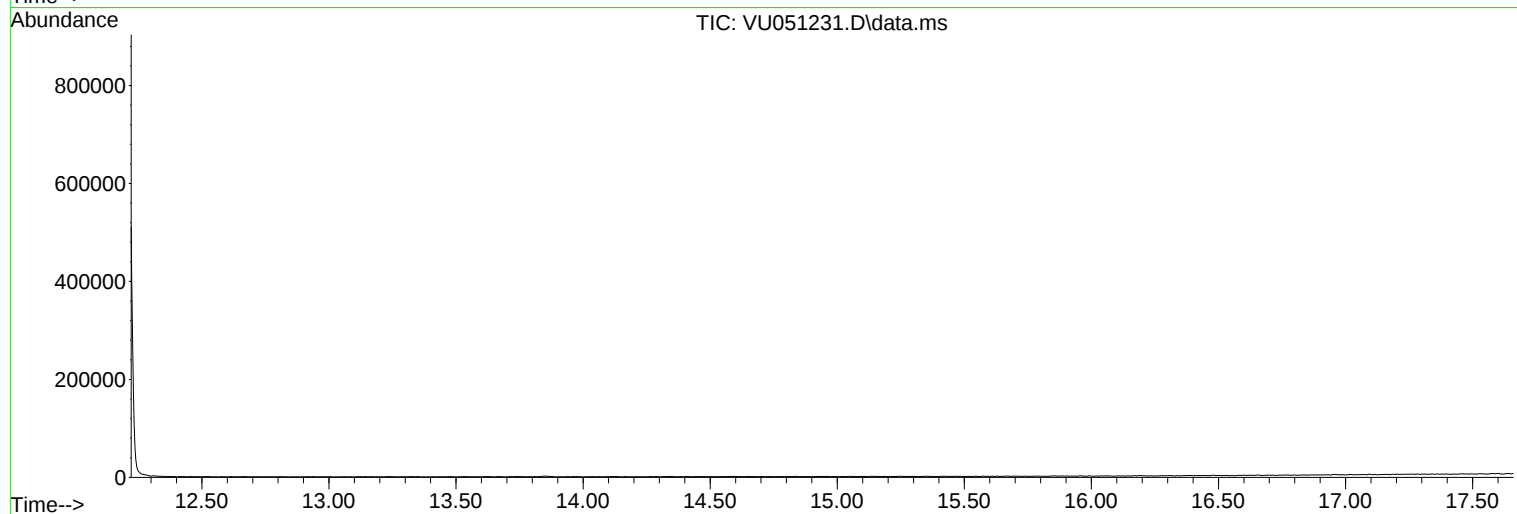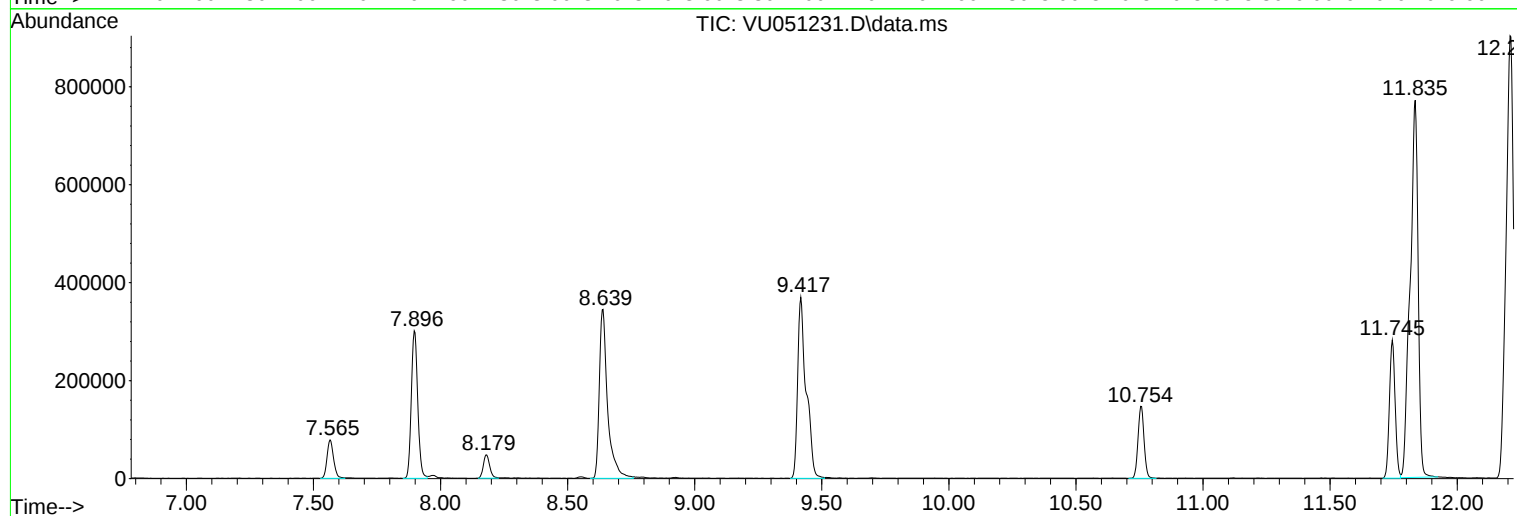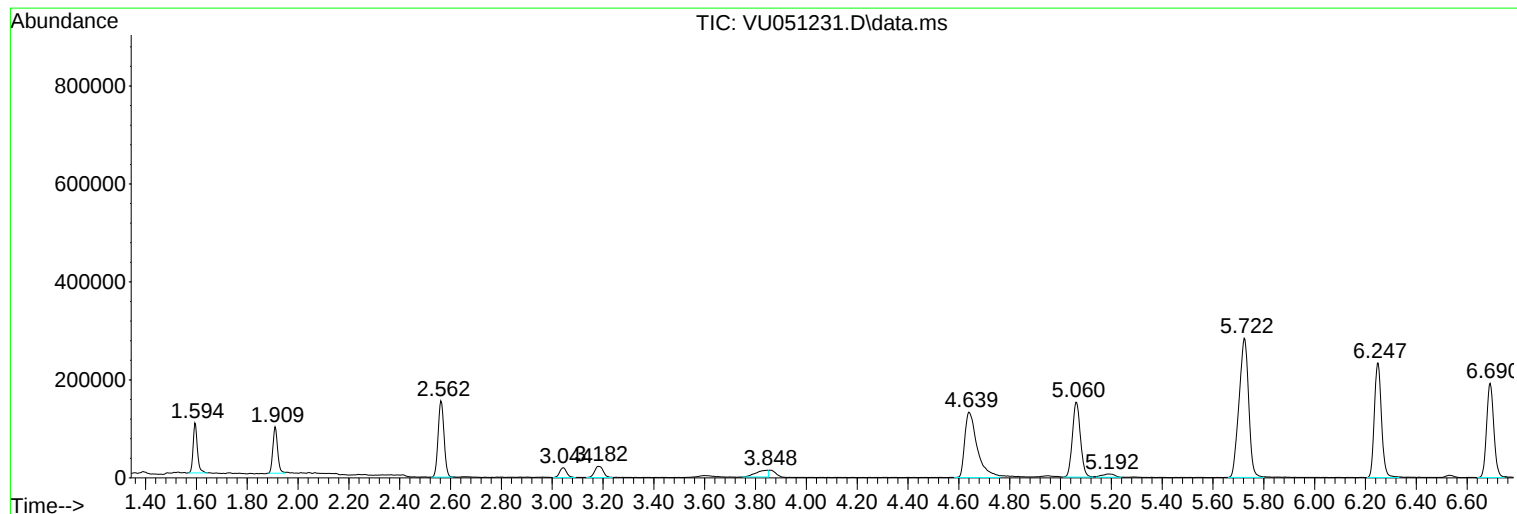

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051231.D
Acq On : 07 Oct 2022 20:37
Operator : JC/MD
Sample : N4872-12DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXFX6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051231.D
Acq On : 07 Oct 2022 20:37
Operator : JC/MD
Sample : N4872-12DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXFX6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc