

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051251.D
 Acq On : 08 Oct 2022 05:17
 Operator : JC/MD
 Sample : N4899-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5H53

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051251.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	87	rBV	93693	122975	18.51%	2.380%
2	1.909	170	177	189	rVB	74142	99076	14.92%	1.917%
3	2.565	369	381	394	rBV	114306	186565	28.09%	3.610%
4	3.183	562	573	588	rBV	7005	13512	2.03%	0.261%
5	3.851	752	781	805	rVB2	23523	91419	13.76%	1.769%
6	4.623	1008	1021	1045	rBV	109911	281300	42.35%	5.443%
7	5.063	1142	1158	1178	rBV	129423	285585	42.99%	5.526%
8	5.199	1182	1200	1202	rVV	7904	17751	2.67%	0.343%
9	5.215	1202	1205	1221	rVB	9871	17084	2.57%	0.331%
10	5.726	1343	1364	1394	rBV2	230823	628532	94.63%	12.162%
11	6.247	1507	1526	1548	rBV	193560	375442	56.52%	7.265%
12	6.690	1647	1664	1683	rBV	165289	328924	49.52%	6.365%
13	7.565	1920	1936	1949	rBV3	61976	109595	16.50%	2.121%
14	7.896	2026	2039	2055	rBV	238963	415192	62.51%	8.034%
15	7.970	2056	2062	2075	rVB2	7350	12449	1.87%	0.241%
16	8.179	2117	2127	2141	rBV	39764	65739	9.90%	1.272%
17	8.632	2255	2268	2305	rBV2	294205	664231	100.00%	12.853%
18	9.417	2497	2512	2540	rBV	317604	527973	79.49%	10.216%
19	10.755	2915	2928	2949	rBV	132850	213108	32.08%	4.124%
20	11.812	3243	3257	3281	rBV	222853	365539	55.03%	7.073%
21	12.192	3359	3375	3397	rBV	205951	346069	52.10%	6.696%




Sum of corrected areas: 5168060

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051251.D
Acq On : 08 Oct 2022 05:17
Operator : JC/MD
Sample : N4899-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

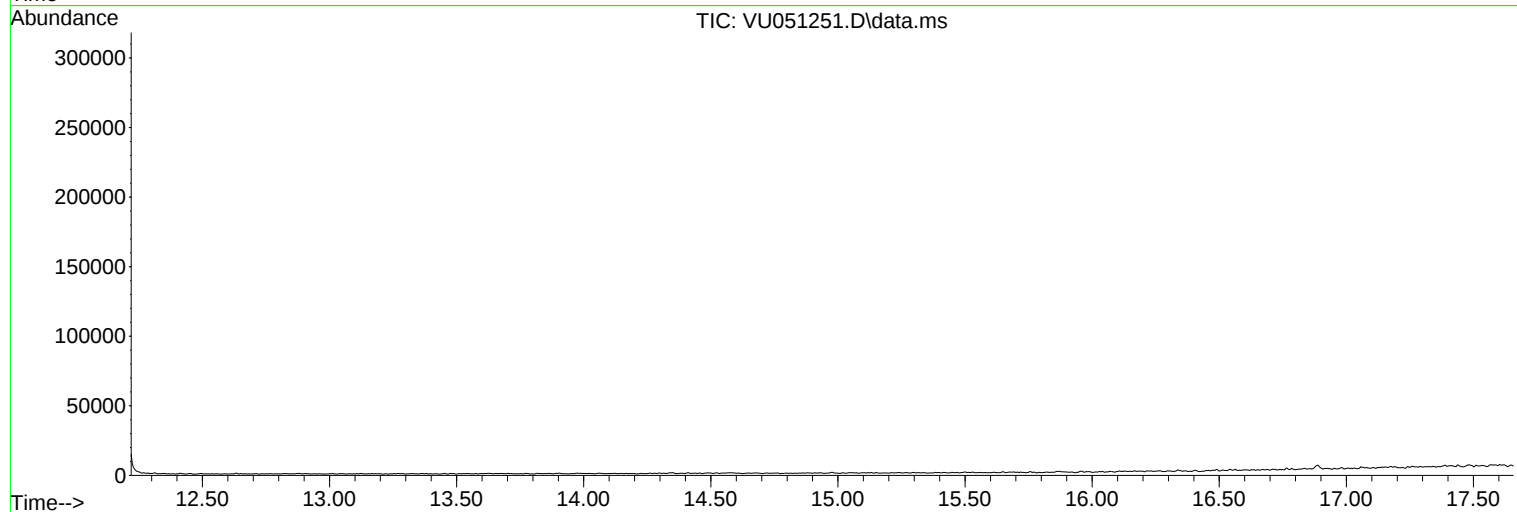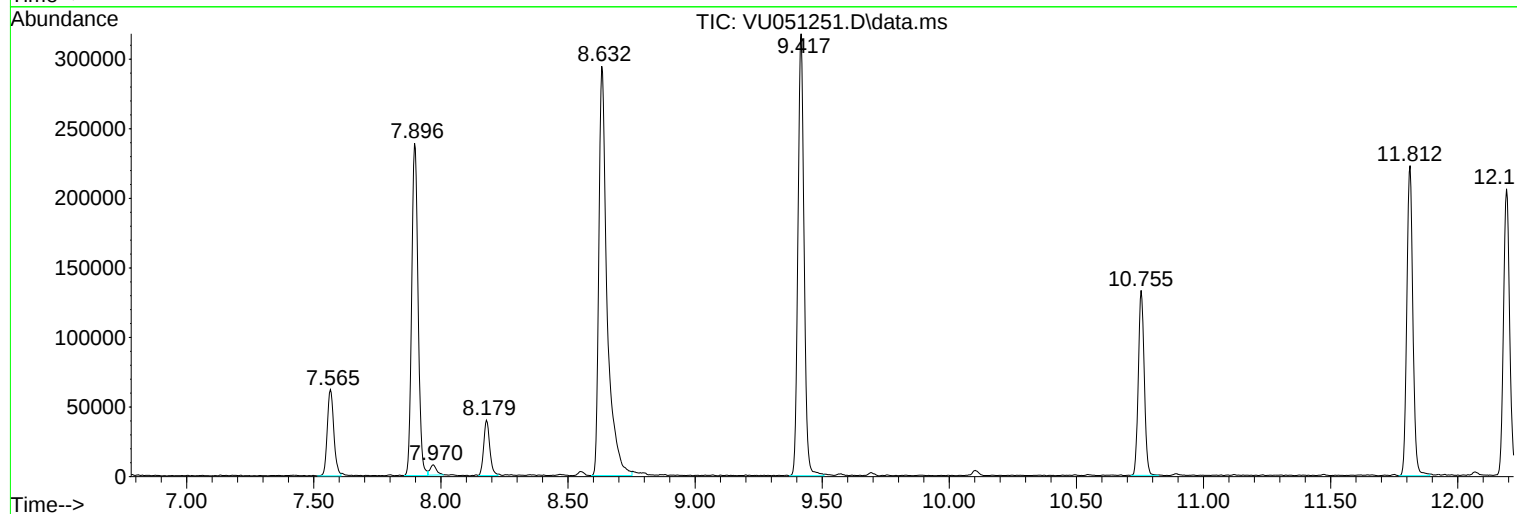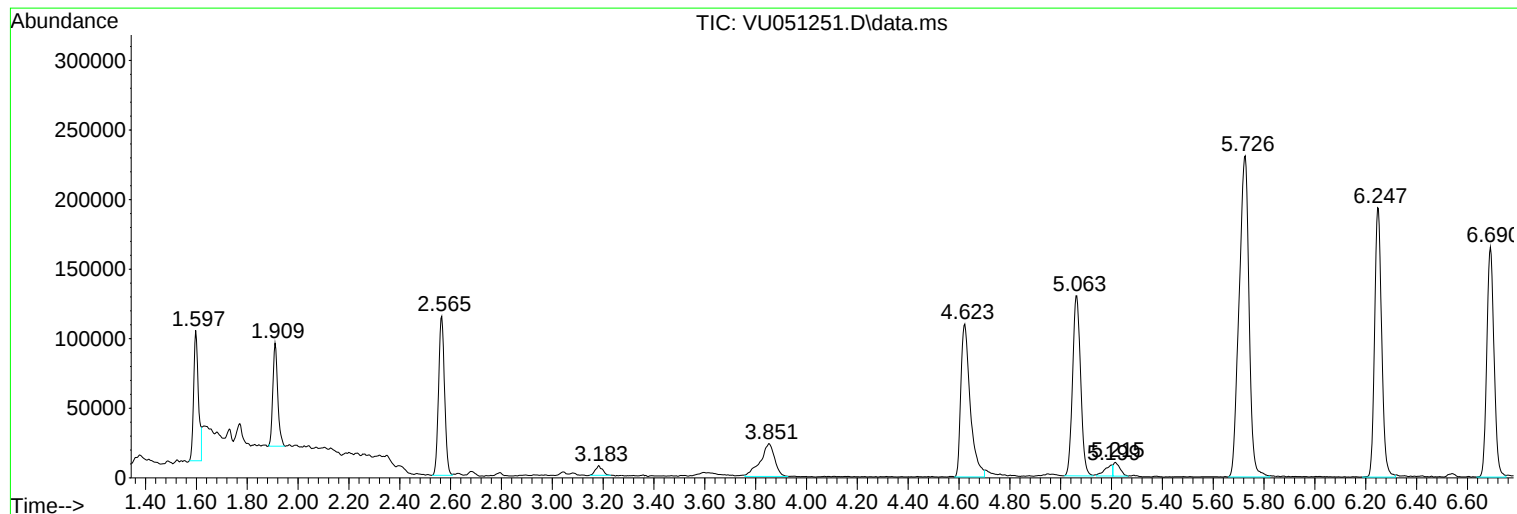

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051251.D
Acq On : 08 Oct 2022 05:17
Operator : JC/MD
Sample : N4899-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H53










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.851	1.22 ug/L	91419	1,4-Difluorobenzene	6.250

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethylenediamine	60	C2H8N2	000107-15-3	4
2			Acetonitrile-d3	44	C2D3N	002206-26-0	4
3			Ethanamine, N-methyl-	59	C3H9N	000624-78-2	3
4			2-Propanamine	59	C3H9N	000075-31-0	3
5			Ethylene oxide	44	C2H4O	000075-21-8	3

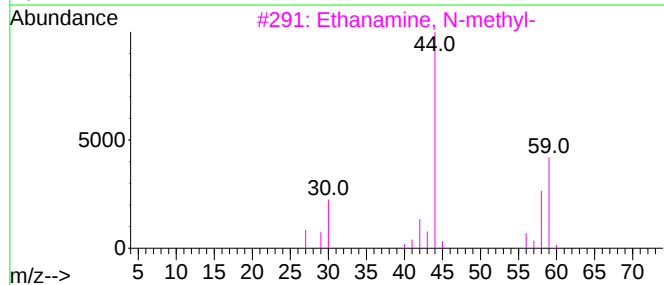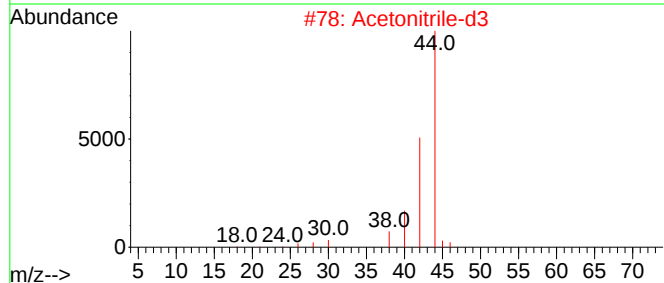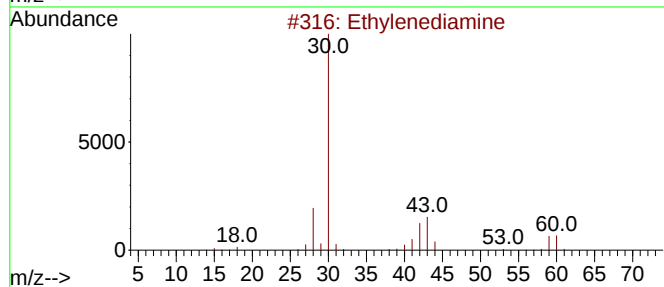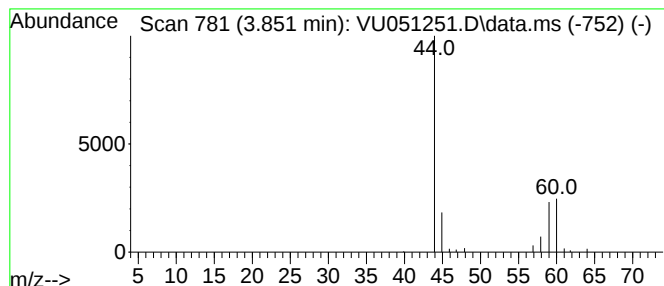

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051251.D
Acq On : 08 Oct 2022 05:17
Operator : JC/MD
Sample : N4899-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.851	1.2	ug/L	91419	1	6.250	375442	5.0