

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051262.D
 Acq On : 08 Oct 2022 09:49
 Operator : JC/MD
 Sample : N4931-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5H18

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051262.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	80350	92558	13.39%	1.755%
2	1.729	115	121	127	rBV	21903	25900	3.75%	0.491%
3	1.912	170	178	189	rVB	75894	98656	14.28%	1.870%
4	2.565	367	381	396	rBV	121697	196515	28.44%	3.725%
5	3.182	559	573	592	rBV2	7514	17160	2.48%	0.325%
6	3.835	754	776	794	rVB	7194	25490	3.69%	0.483%
7	4.623	1007	1021	1061	rBV2	113462	305648	44.23%	5.794%
8	5.060	1142	1157	1175	rBV	130251	286897	41.51%	5.439%
9	5.726	1343	1364	1391	rBV2	228311	623174	90.18%	11.813%
10	6.247	1513	1526	1548	rBV	211829	414071	59.92%	7.850%
11	6.690	1651	1664	1687	rBV	164217	322323	46.64%	6.110%
12	7.565	1925	1936	1956	rBV2	62132	110134	15.94%	2.088%
13	7.896	2024	2039	2055	rBV	232759	411092	59.49%	7.793%
14	7.970	2056	2062	2076	rVB3	4604	7706	1.12%	0.146%
15	8.179	2115	2127	2144	rBV2	37289	64607	9.35%	1.225%
16	8.636	2255	2269	2310	rBV4	289531	691069	100.00%	13.101%
17	9.417	2498	2512	2530	rBV	349247	583840	84.48%	11.068%
18	10.754	2916	2928	2948	rBV	134040	222980	32.27%	4.227%
19	11.812	3245	3257	3278	rBV	260897	418001	60.49%	7.924%
20	12.192	3363	3375	3398	rBV	214329	357284	51.70%	6.773%




Sum of corrected areas: 5275105

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051262.D
Acq On : 08 Oct 2022 09:49
Operator : JC/MD
Sample : N4931-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

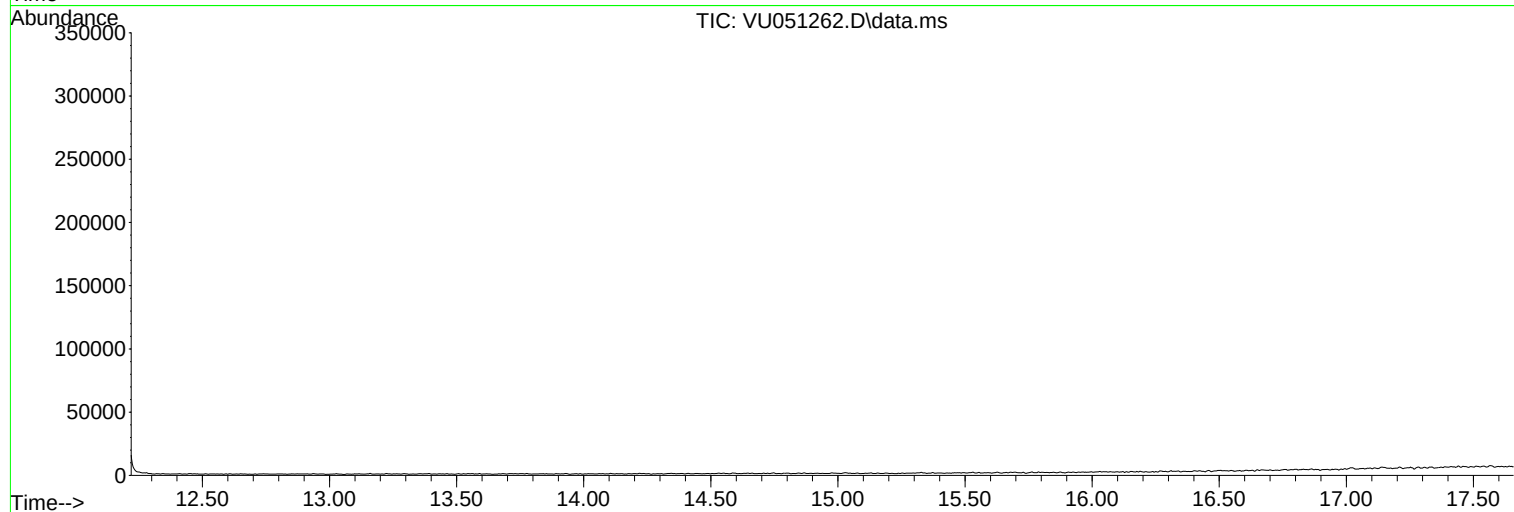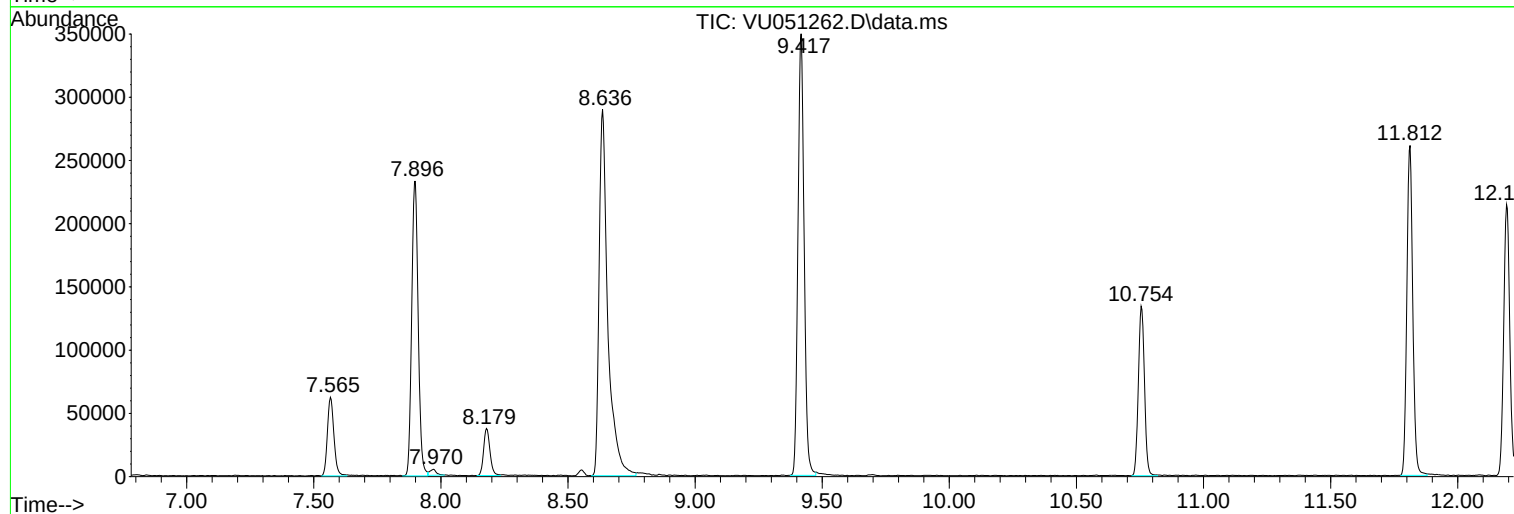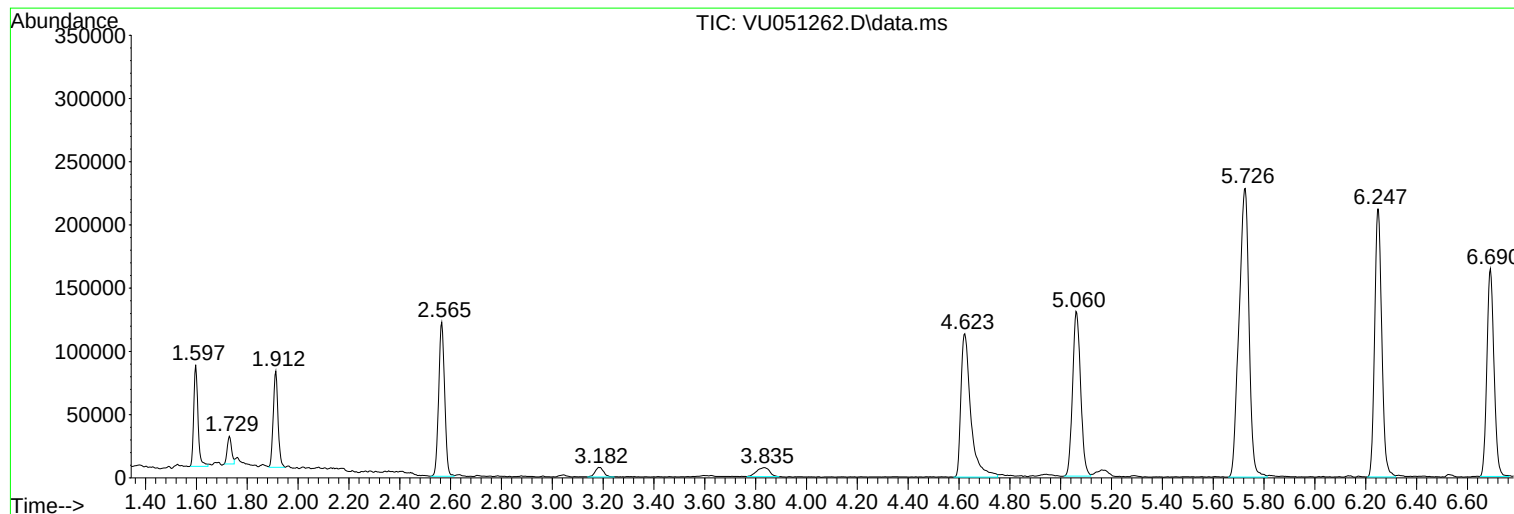

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051262.D
Acq On : 08 Oct 2022 09:49
Operator : JC/MD
Sample : N4931-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051262.D
Acq On : 08 Oct 2022 09:49
Operator : JC/MD
Sample : N4931-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc