

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051263.D
 Acq On : 08 Oct 2022 10:14
 Operator : JC/MD
 Sample : N4931-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5H19

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	73	79	98	rVB	78216	93781	12.59%	1.750%
2	1.729	115	121	130	rVB	14490	17084	2.29%	0.319%
3	1.909	170	177	192	rVB	76641	97768	13.12%	1.824%
4	2.565	369	381	396	rBV	119770	194255	26.07%	3.624%
5	3.829	755	774	794	rVB	6364	22732	3.05%	0.424%
6	4.623	1009	1021	1057	rBV2	118719	316081	42.42%	5.897%
7	5.060	1141	1157	1175	rBV	134306	296299	39.76%	5.528%
8	5.723	1341	1363	1380	rBV2	239520	640613	85.97%	11.952%
9	6.247	1511	1526	1547	rBV	194965	373712	50.15%	6.972%
10	6.690	1650	1664	1682	rBV	172385	334575	44.90%	6.242%
11	7.565	1924	1936	1949	rBV2	64088	113453	15.23%	2.117%
12	7.896	2026	2039	2055	rBV	245166	425460	57.10%	7.938%
13	7.964	2056	2060	2076	rVB4	5046	9279	1.25%	0.173%
14	8.179	2117	2127	2147	rBV	41312	70651	9.48%	1.318%
15	8.636	2256	2269	2302	rBV2	327763	745157	100.00%	13.903%
16	9.417	2498	2512	2534	rBV	320110	536700	72.03%	10.013%
17	10.031	2694	2703	2712	rBV6	5755	9924	1.33%	0.185%
18	10.359	2795	2805	2819	rVB6	3599	8938	1.20%	0.167%
19	10.755	2916	2928	2942	rBV2	144246	234526	31.47%	4.376%
20	11.809	3241	3256	3275	rBV	254743	415847	55.81%	7.759%
21	12.192	3359	3375	3402	rBV2	243810	402965	54.08%	7.518%




Sum of corrected areas: 5359800

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051263.D
Acq On : 08 Oct 2022 10:14
Operator : JC/MD
Sample : N4931-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

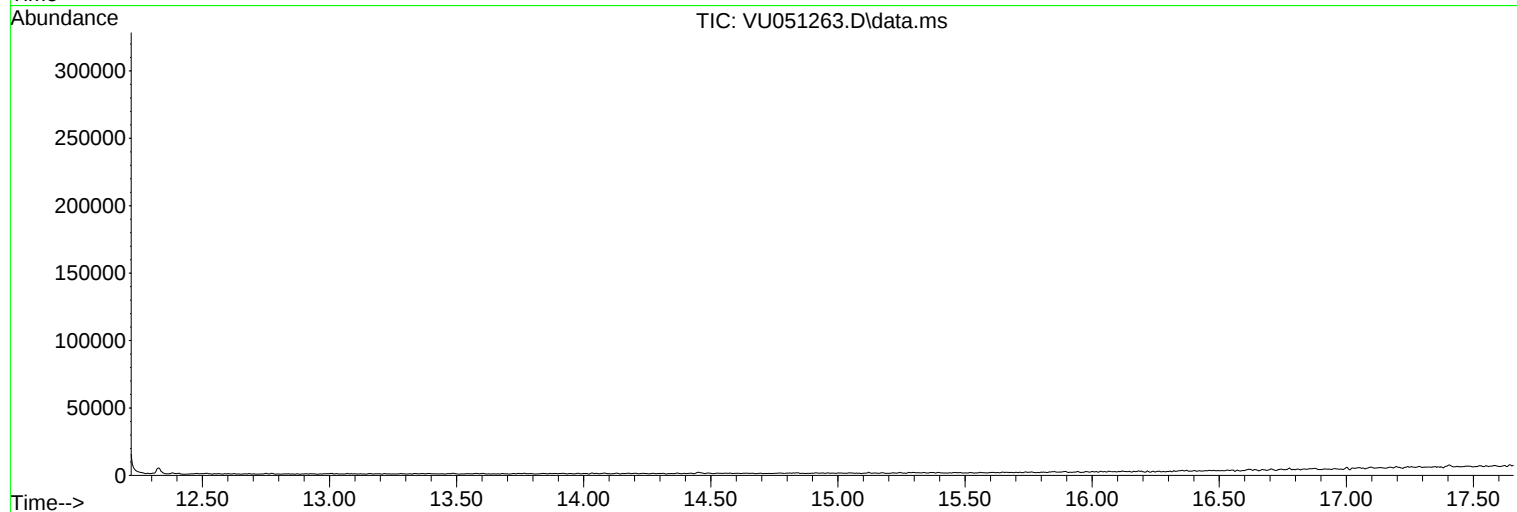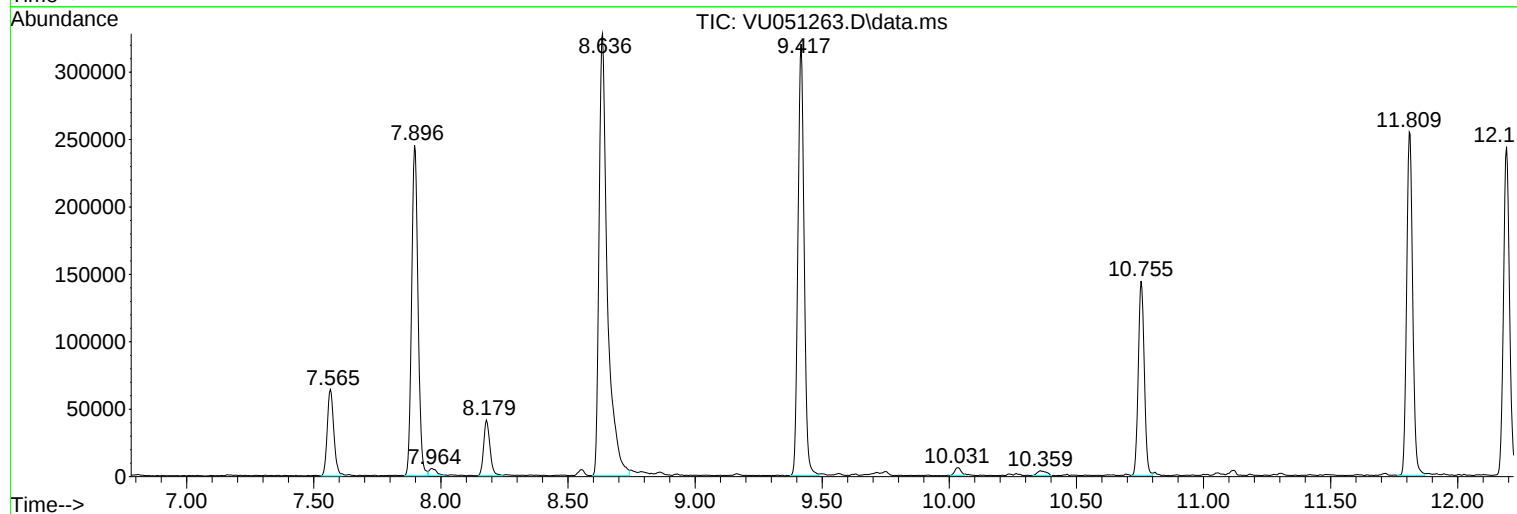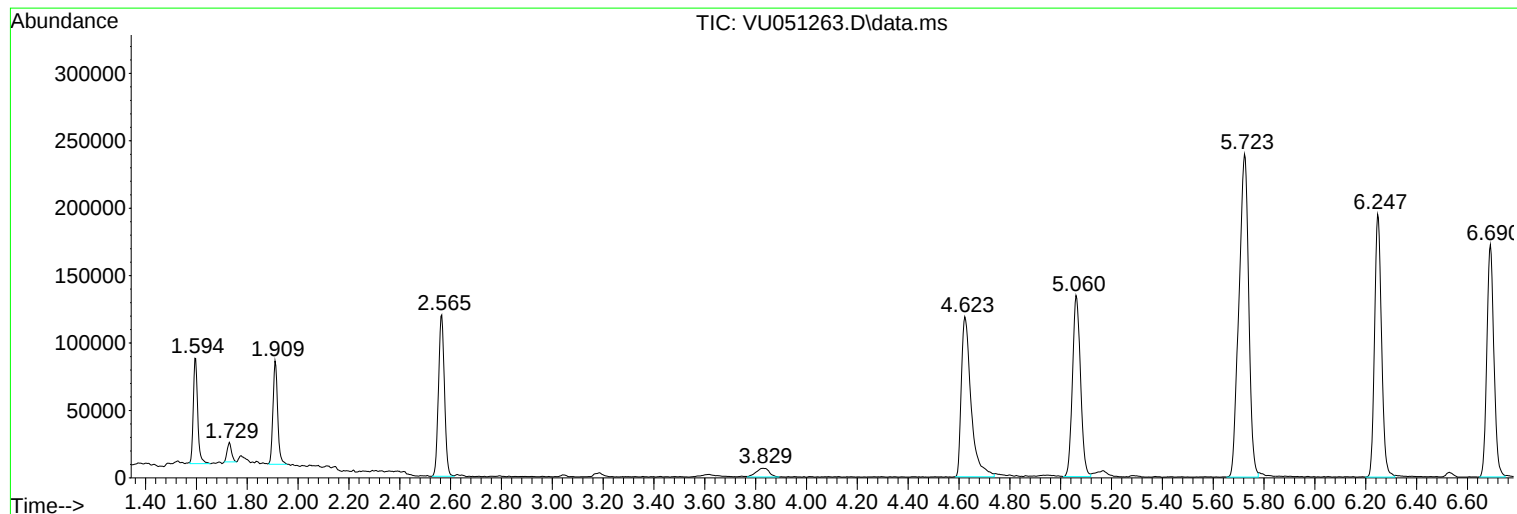

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051263.D
Acq On : 08 Oct 2022 10:14
Operator : JC/MD
Sample : N4931-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051263.D
Acq On : 08 Oct 2022 10:14
Operator : JC/MD
Sample : N4931-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc