

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051270.D
 Acq On : 08 Oct 2022 14:26
 Operator : JC/MD
 Sample : N5064-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BT6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051270.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	102	rVB	87208	104064	14.97%	1.924%
2	1.913	169	178	190	rBV	82419	108710	15.64%	2.009%
3	2.565	369	381	399	rVB	134852	217688	31.31%	4.024%
4	3.832	758	775	776	rBV2	6498	12530	1.80%	0.232%
5	4.646	1014	1028	1070	rBV2	84273	307303	44.20%	5.680%
6	5.064	1143	1158	1181	rBV	145307	328658	47.27%	6.075%
7	5.186	1185	1196	1214	rVB	7592	22338	3.21%	0.413%
8	5.726	1342	1364	1387	rBV2	260262	681463	98.01%	12.596%
9	6.250	1513	1527	1552	rBV	202358	388918	55.94%	7.189%
10	6.530	1605	1614	1623	rVB5	4213	7566	1.09%	0.140%
11	6.690	1650	1664	1683	rBV	180608	351547	50.56%	6.498%
12	7.565	1924	1936	1954	rBV	65559	118032	16.98%	2.182%
13	7.896	2024	2039	2054	rBV	255715	451289	64.91%	8.342%
14	7.970	2055	2062	2073	rVB2	7750	13634	1.96%	0.252%
15	8.182	2115	2128	2147	rBV	39508	69956	10.06%	1.293%
16	8.639	2256	2270	2307	rBV3	278285	695295	100.00%	12.852%
17	9.417	2497	2512	2535	rBV	316713	537349	77.28%	9.933%
18	10.755	2915	2928	2946	rBV	133911	221228	31.82%	4.089%
19	11.812	3245	3257	3277	rBV	240414	392150	56.40%	7.249%
20	12.192	3357	3375	3393	rBV	230887	380222	54.68%	7.028%




Sum of corrected areas: 5409940

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051270.D
Acq On : 08 Oct 2022 14:26
Operator : JC/MD
Sample : N5064-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 62 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

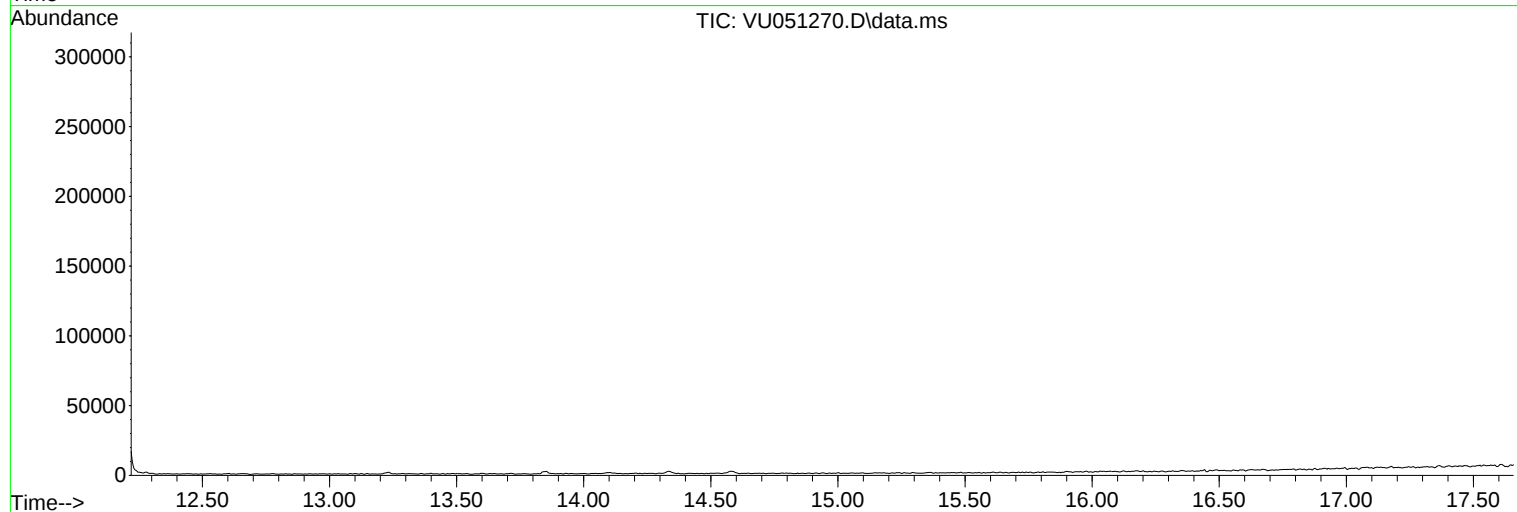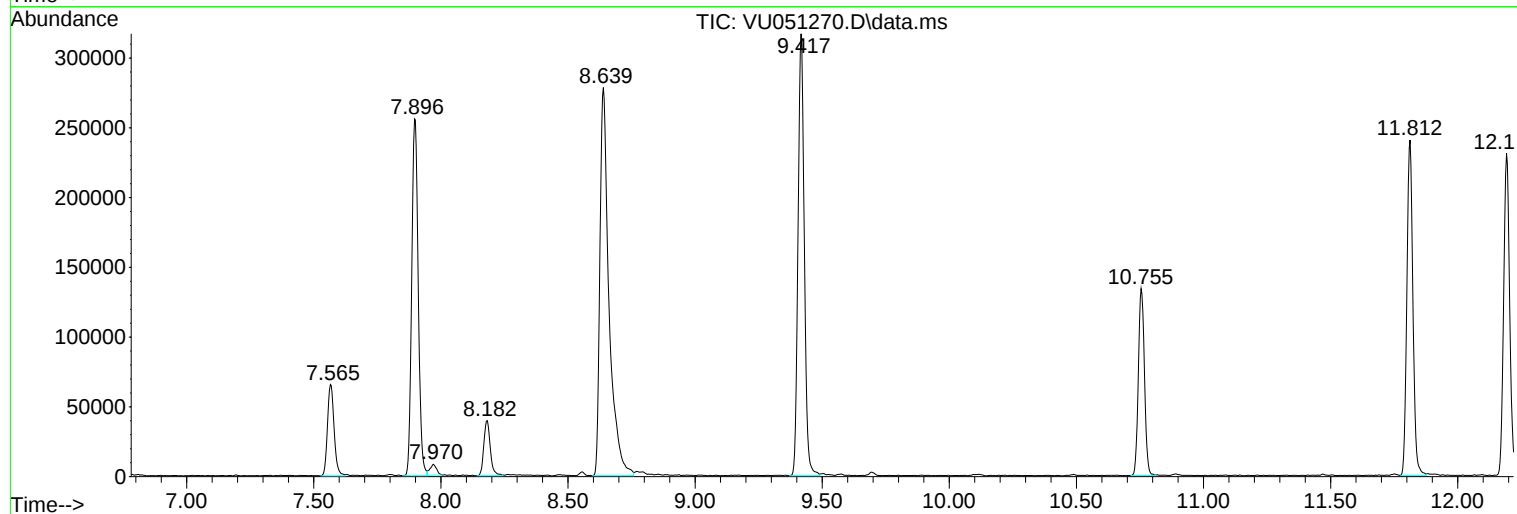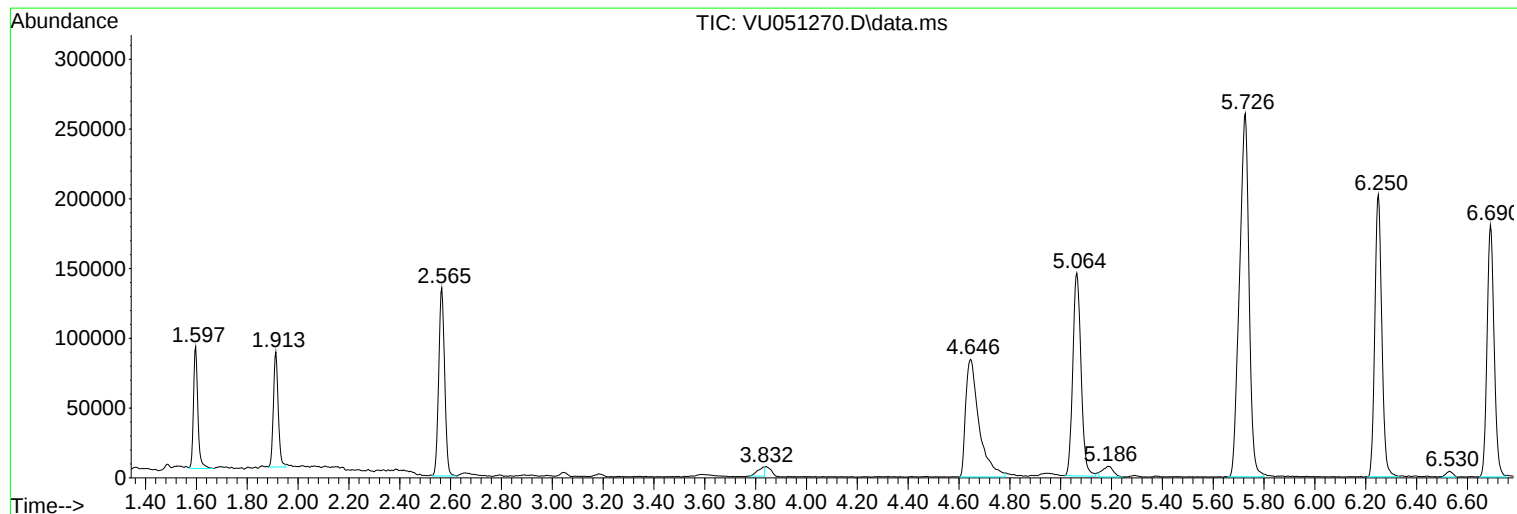

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051270.D
Acq On : 08 Oct 2022 14:26
Operator : JC/MD
Sample : N5064-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 62 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051270.D
Acq On : 08 Oct 2022 14:26
Operator : JC/MD
Sample : N5064-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 62 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc