

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051271.D
 Acq On : 08 Oct 2022 14:51
 Operator : JC/MD
 Sample : N5049-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BT5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051271.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	93	rBV	75864	88483	12.07%	1.634%
2	1.912	170	178	192	rBV	74767	96039	13.10%	1.773%
3	2.565	368	381	399	rBV	117307	192811	26.30%	3.560%
4	2.658	399	410	414	rBV2	4405	8699	1.19%	0.161%
5	3.845	758	779	798	rVB	7480	25231	3.44%	0.466%
6	4.642	1011	1027	1066	rBV	91949	326882	44.58%	6.035%
7	5.060	1141	1157	1177	rBV2	135327	311271	42.45%	5.747%
8	5.726	1341	1364	1383	rBV3	241617	642687	87.65%	11.865%
9	6.247	1512	1526	1543	rBV	215894	413978	56.46%	7.643%
10	6.690	1649	1664	1684	rBV	172525	336716	45.92%	6.216%
11	7.565	1925	1936	1950	rBV	62632	110008	15.00%	2.031%
12	7.896	2026	2039	2055	rBV	244179	424365	57.88%	7.835%
13	7.970	2057	2062	2078	rVB4	6194	11425	1.56%	0.211%
14	8.179	2115	2127	2144	rBV2	38292	67887	9.26%	1.253%
15	8.639	2257	2270	2307	rBV4	301742	733230	100.00%	13.537%
16	9.417	2498	2512	2534	rBV	343784	584389	79.70%	10.789%
17	10.754	2914	2928	2943	rBV	136136	222633	30.36%	4.110%
18	10.890	2963	2970	2982	rVB3	5245	7931	1.08%	0.146%
19	11.812	3241	3257	3279	rBV	265618	432251	58.95%	7.980%
20	12.192	3363	3375	3396	rBV	234735	379623	51.77%	7.009%




Sum of corrected areas: 5416539

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051271.D
Acq On : 08 Oct 2022 14:51
Operator : JC/MD
Sample : N5049-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 63 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

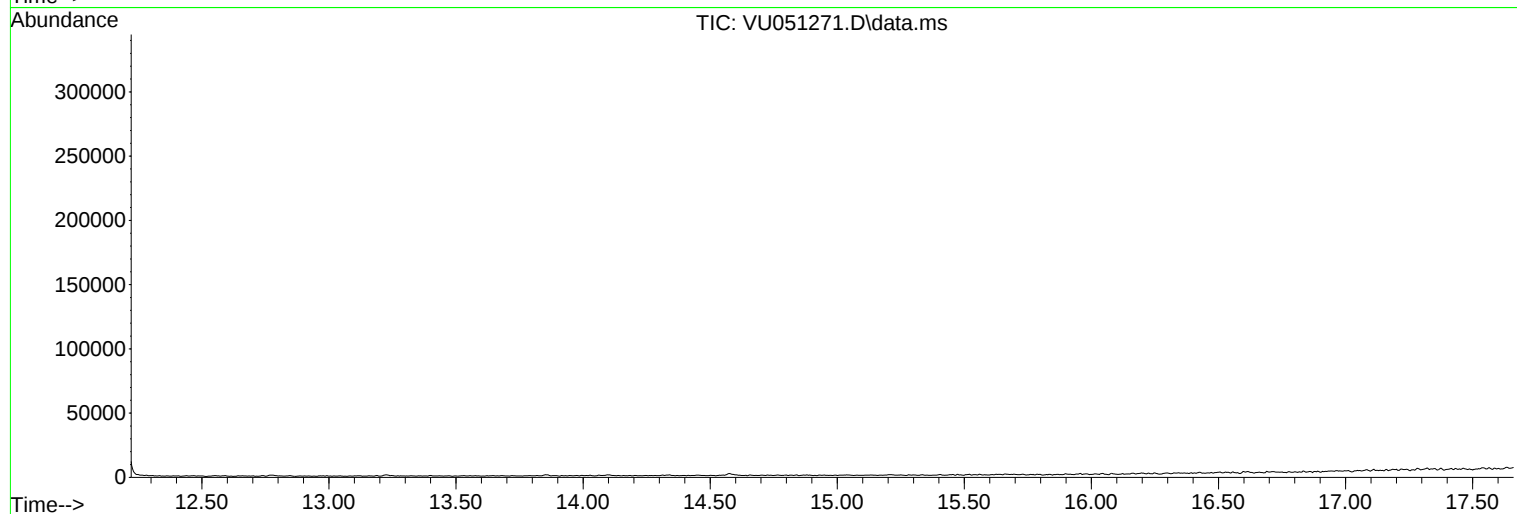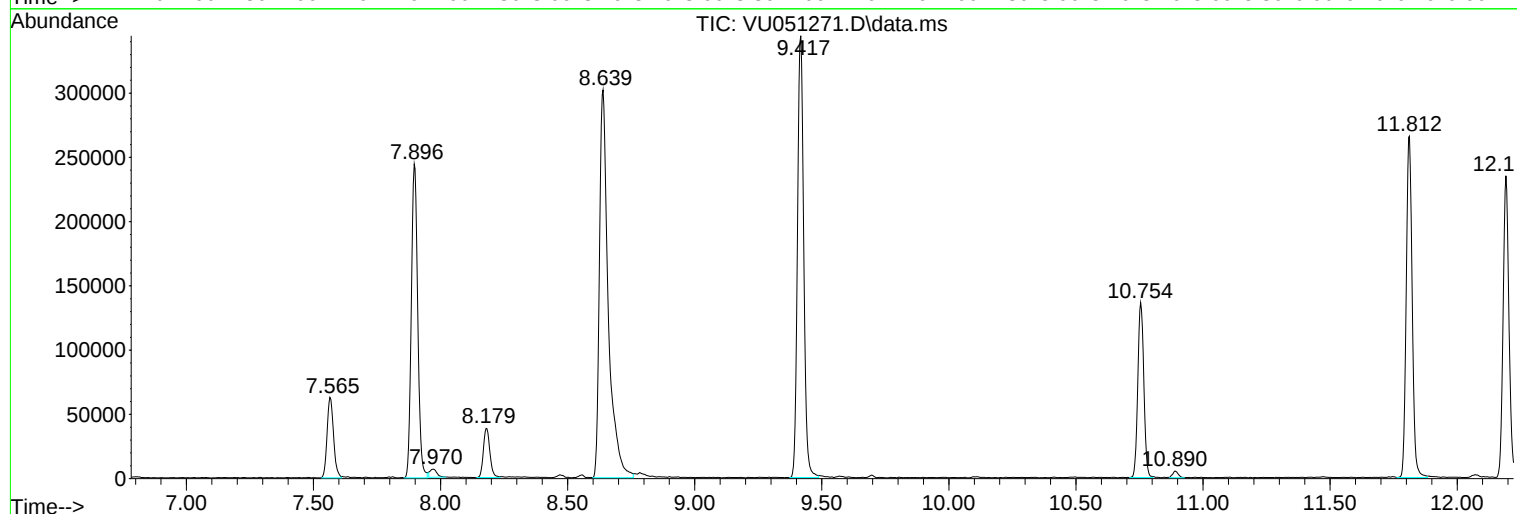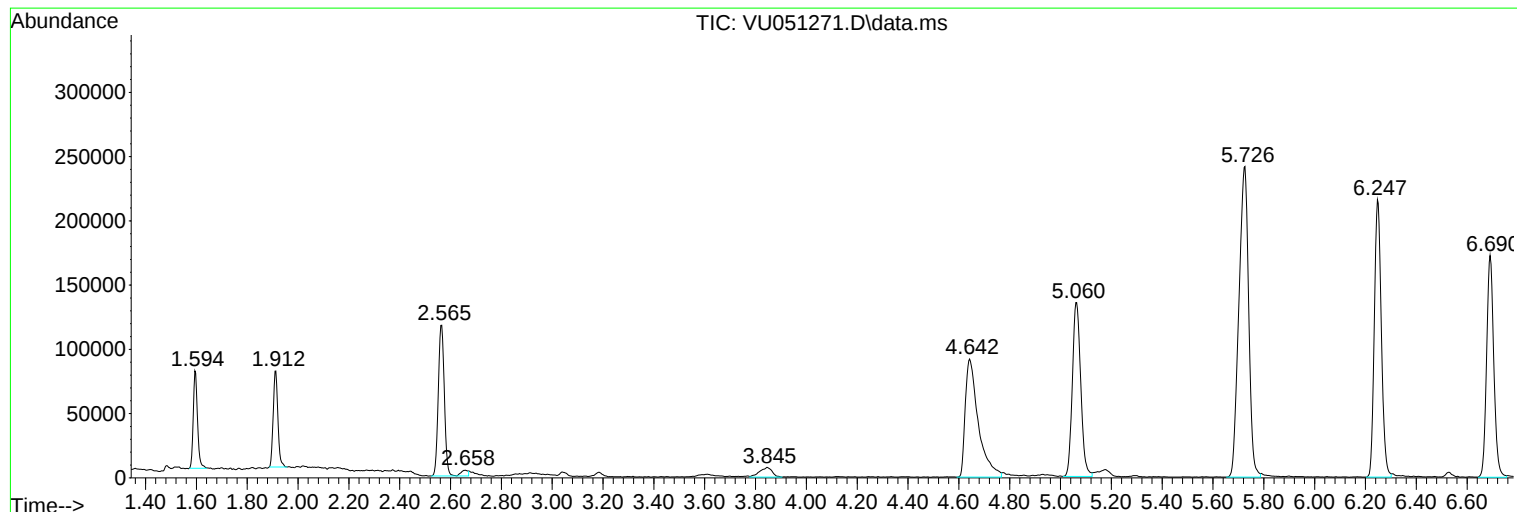

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051271.D
Acq On : 08 Oct 2022 14:51
Operator : JC/MD
Sample : N5049-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 63 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.565	1.33 ug/L	110008	1,4-Difluorobenzene	6.247

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	38
2			Thiophosgene	114	CCl2S	000463-71-8	33
3			2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	9
4			2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	9
5			Methanesulfonyl chloride	114	CH3ClO2S	000124-63-0	9

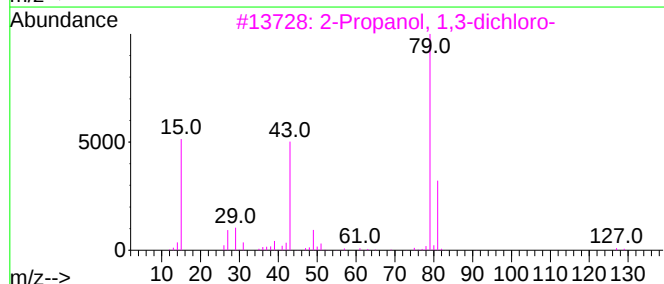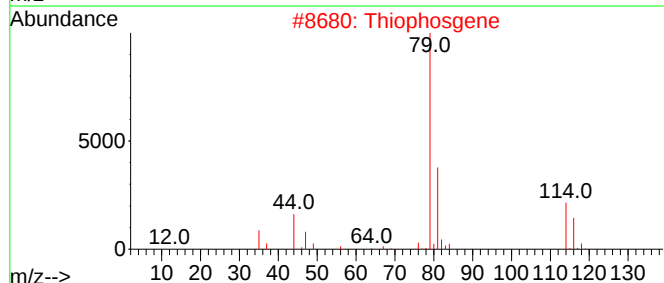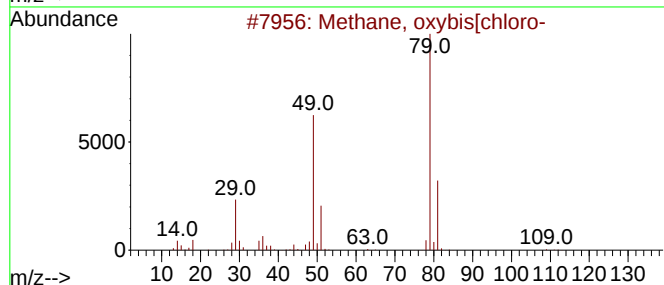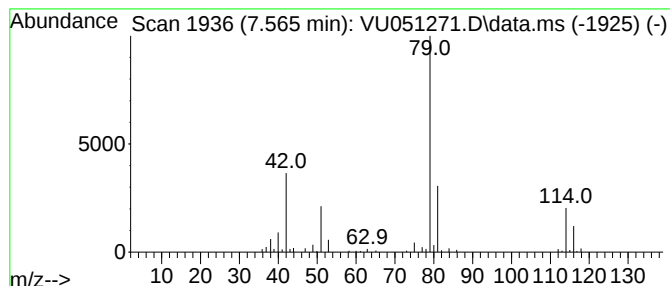

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051271.D
Acq On : 08 Oct 2022 14:51
Operator : JC/MD
Sample : N5049-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 63 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.565	1.3	ug/L	110008	1	6.247	413978	5.0