

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051281.D
 Acq On : 08 Oct 2022 18:56
 Operator : JC/MD
 Sample : N4922-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CB8R1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rBV	82877	95350	13.89%	1.733%
2	1.764	128	132	147	rVB5	12417	17569	2.56%	0.319%
3	1.912	170	178	192	rVB	80201	105724	15.40%	1.922%
4	2.565	369	381	393	rBV	123211	199372	29.04%	3.624%
5	2.626	393	400	413	rVB2	6043	11488	1.67%	0.209%
6	3.835	749	776	793	rVB	6593	21396	3.12%	0.389%
7	4.623	1008	1021	1051	rBV	105605	281951	41.07%	5.125%
8	5.063	1140	1158	1176	rBV	141423	312706	45.55%	5.684%
9	5.726	1342	1364	1390	rBV3	252971	674329	98.22%	12.257%
10	6.247	1512	1526	1555	rBV	215322	416370	60.64%	7.568%
11	6.690	1650	1664	1681	rBV	178205	348517	50.76%	6.335%
12	7.565	1925	1936	1952	rBV	63499	113229	16.49%	2.058%
13	7.896	2026	2039	2056	rBV	259230	452621	65.92%	8.227%
14	8.179	2115	2127	2143	rBV	41125	68878	10.03%	1.252%
15	8.636	2254	2269	2309	rBV3	286244	686575	100.00%	12.480%
16	8.787	2310	2316	2330	rVB6	5252	9841	1.43%	0.179%
17	9.417	2499	2512	2533	rBV	336090	576600	83.98%	10.481%
18	10.754	2916	2928	2946	rBV	140969	230487	33.57%	4.189%
19	11.812	3244	3257	3276	rBV	267067	434714	63.32%	7.902%
20	12.060	3325	3334	3354	rBV2	20278	38676	5.63%	0.703%
21	12.192	3363	3375	3401	rBV	241167	405186	59.02%	7.365%




Sum of corrected areas: 5501579

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051281.D
Acq On : 08 Oct 2022 18:56
Operator : JC/MD
Sample : N4922-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CB8R1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

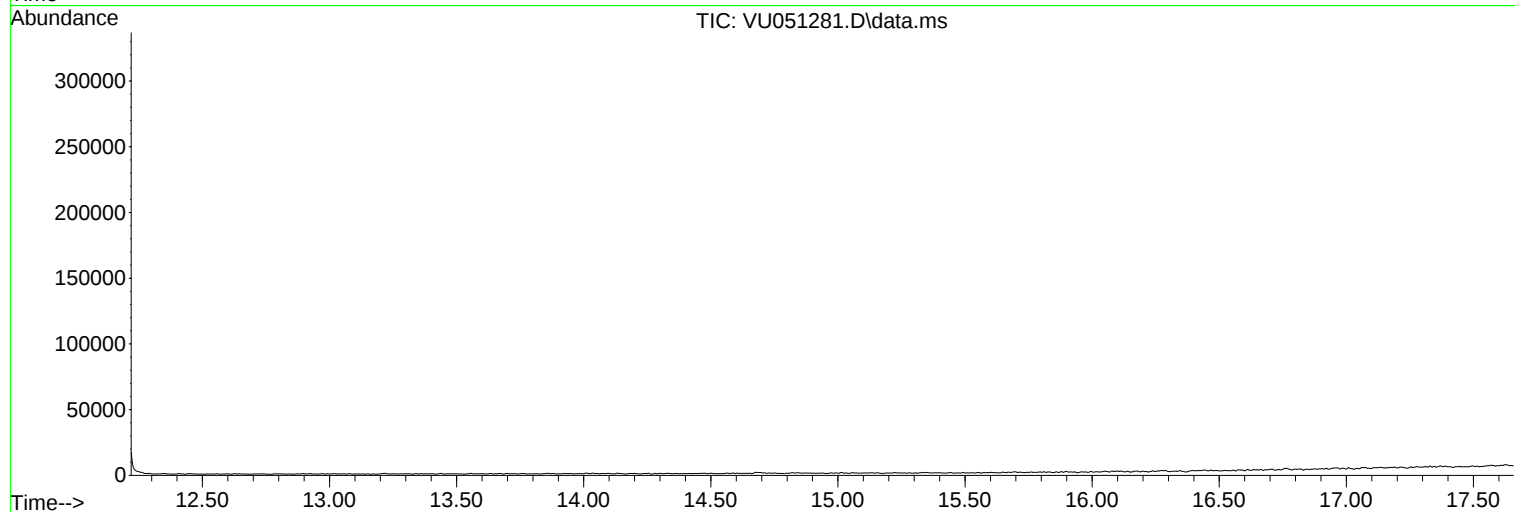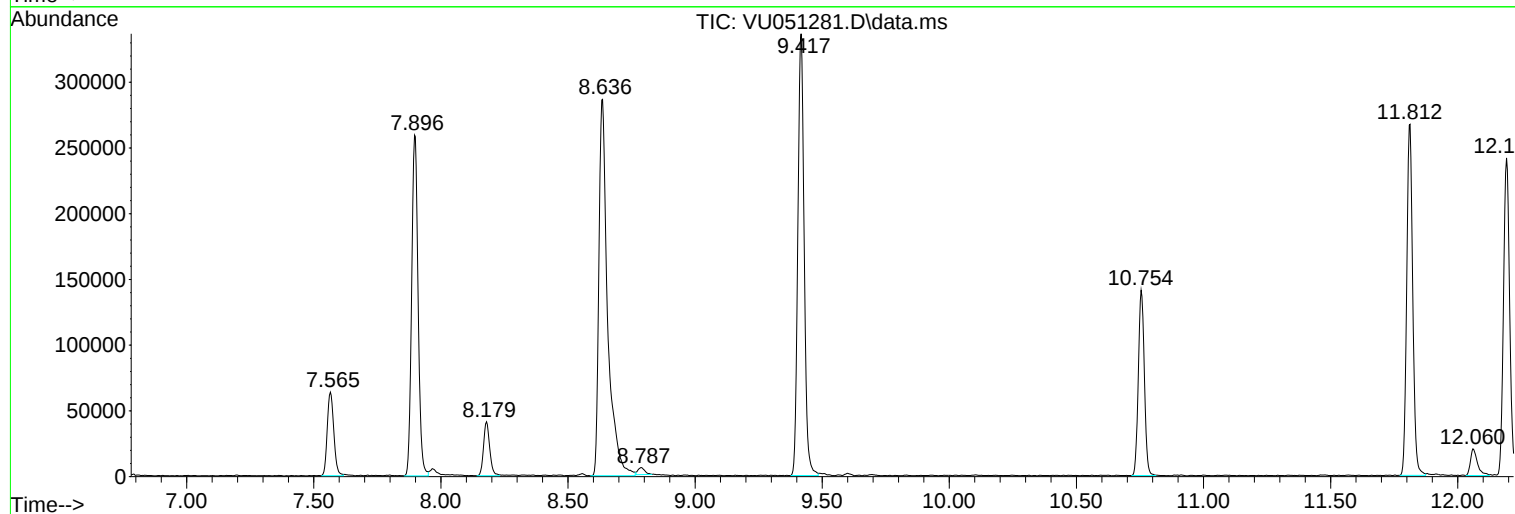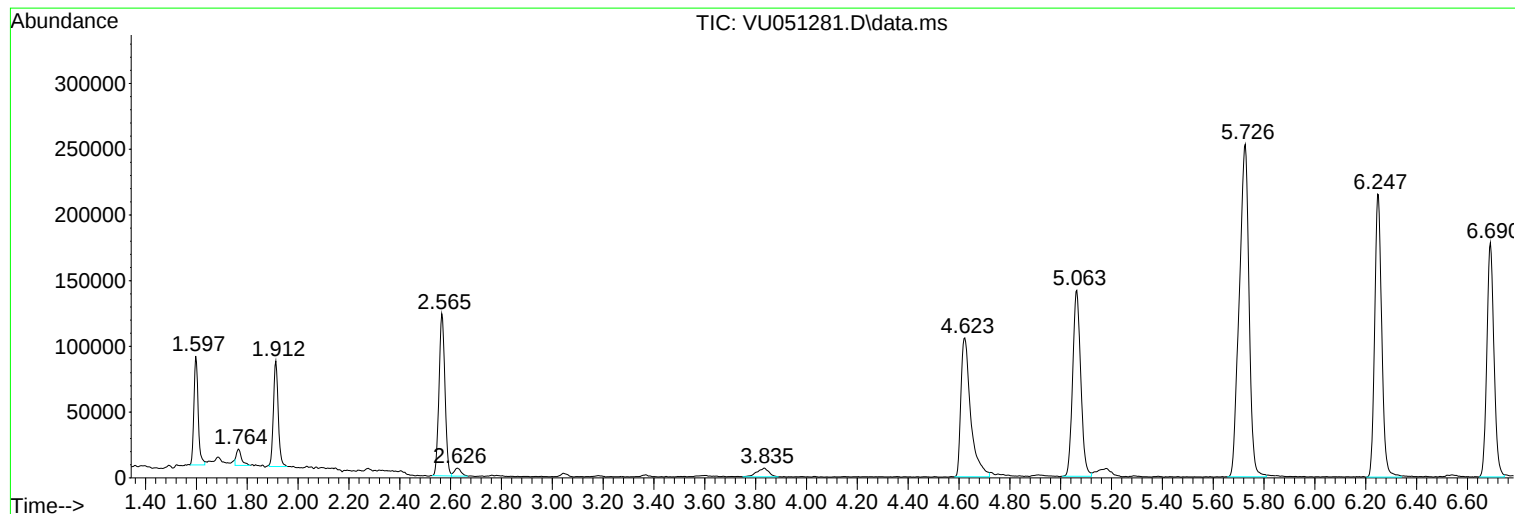

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051281.D
Acq On : 08 Oct 2022 18:56
Operator : JC/MD
Sample : N4922-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CB8R1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051281.D
Acq On : 08 Oct 2022 18:56
Operator : JC/MD
Sample : N4922-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CB8R1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc