

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051288.D
 Acq On : 08 Oct 2022 21:49
 Operator : JC/MD
 Sample : N4900-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXFT0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051288.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rBV	82061	92162	14.23%	1.732%
2	1.764	124	132	140	rBV4	9773	14089	2.18%	0.265%
3	1.912	169	178	194	rBV	77123	100270	15.48%	1.884%
4	2.565	368	381	394	rBV	123337	199645	30.83%	3.752%
5	3.864	764	785	801	rVB	5495	17302	2.67%	0.325%
6	4.623	1009	1021	1052	rBV	99299	260961	40.29%	4.904%
7	5.063	1143	1158	1177	rBV	135508	299158	46.19%	5.622%
8	5.208	1199	1203	1215	rVB	4700	8396	1.30%	0.158%
9	5.726	1343	1364	1384	rBV2	243901	647652	100.00%	12.171%
10	6.250	1512	1527	1543	rBV	209850	404599	62.47%	7.603%
11	6.690	1648	1664	1688	rBV	170340	338055	52.20%	6.353%
12	7.565	1924	1936	1956	rBV2	67294	120582	18.62%	2.266%
13	7.899	2027	2040	2056	rBV	247865	436671	67.42%	8.206%
14	7.967	2056	2061	2075	rVB3	4486	8950	1.38%	0.168%
15	8.179	2117	2127	2148	rBV	41425	71906	11.10%	1.351%
16	8.632	2254	2268	2306	rBV2	266151	644782	99.56%	12.117%
17	9.417	2499	2512	2534	rBV	345834	575789	88.90%	10.820%
18	10.754	2912	2928	2951	rBV	133539	220008	33.97%	4.134%
19	11.812	3244	3257	3273	rBV	271992	439928	67.93%	8.267%
20	12.063	3320	3335	3349	rBV4	15091	29129	4.50%	0.547%
21	12.192	3363	3375	3394	rBV	239658	391451	60.44%	7.356%




Sum of corrected areas: 5321485

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051288.D
Acq On : 08 Oct 2022 21:49
Operator : JC/MD
Sample : N4900-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXFT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

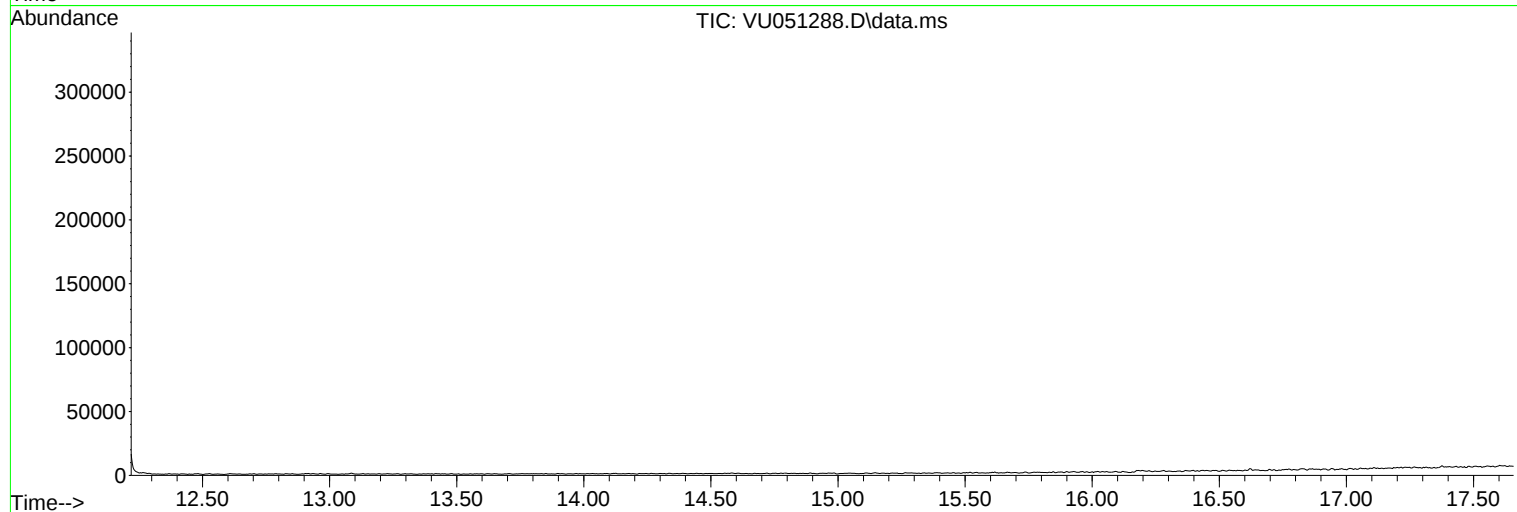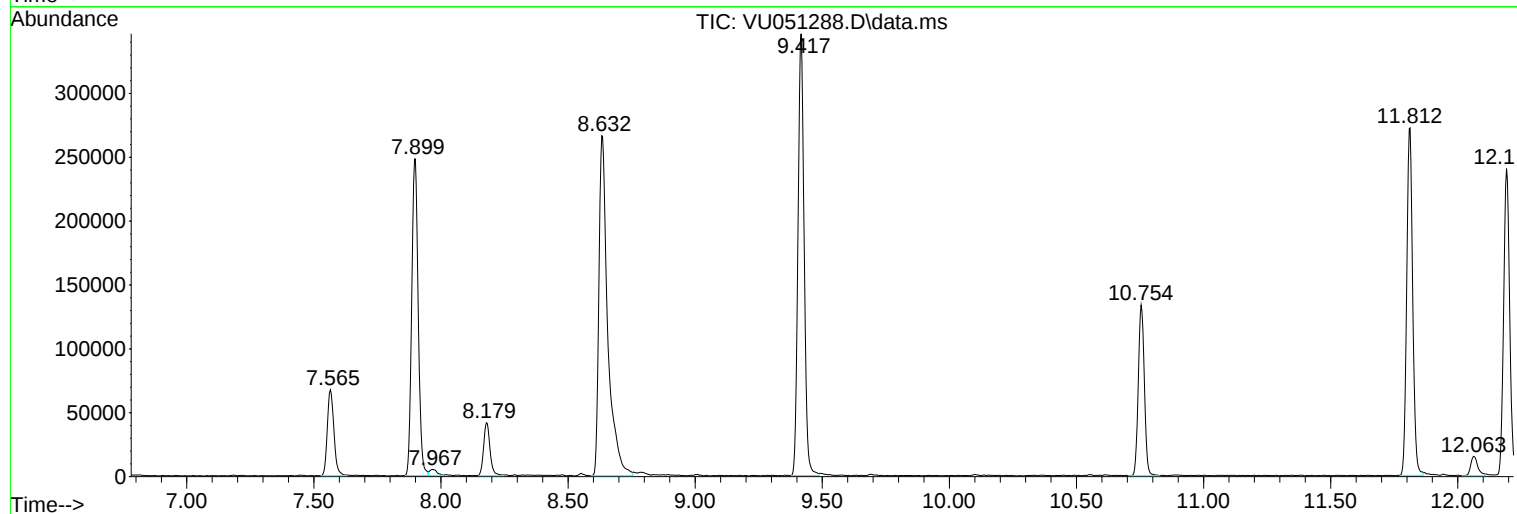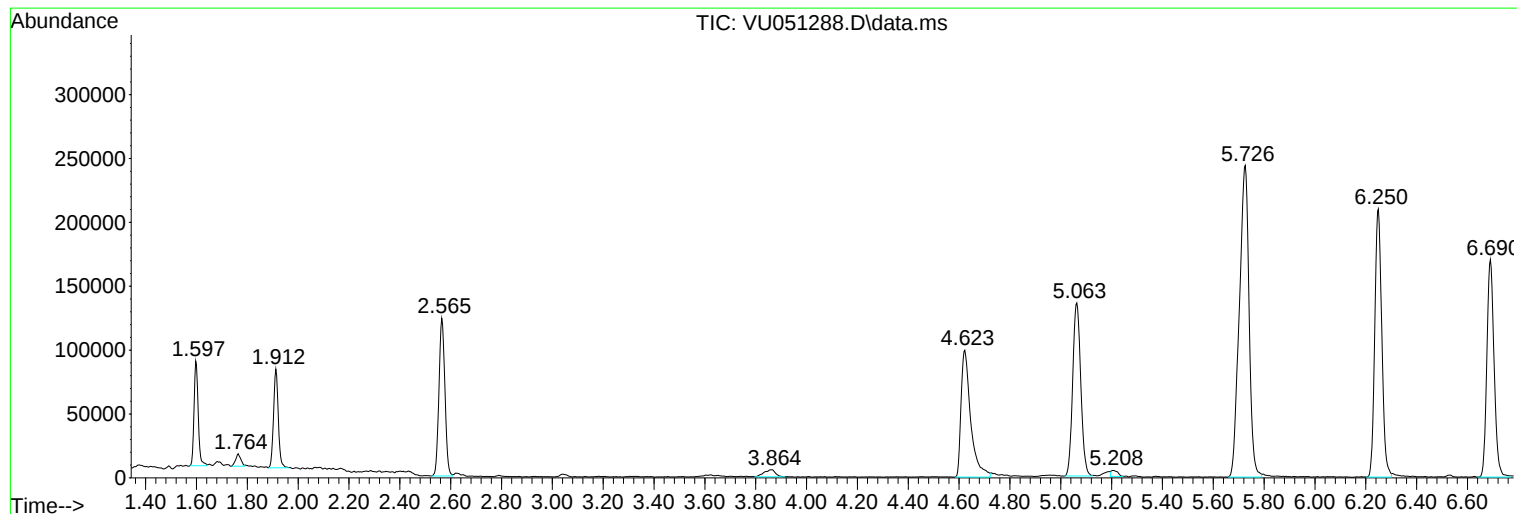

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051288.D
Acq On : 08 Oct 2022 21:49
Operator : JC/MD
Sample : N4900-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXFT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051288.D
Acq On : 08 Oct 2022 21:49
Operator : JC/MD
Sample : N4900-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXFT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------