

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051290.D
 Acq On : 08 Oct 2022 22:38
 Operator : JC/MD
 Sample : N4931-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5H05

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051290.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	83893	96605	13.60%	1.710%
2	1.729	114	121	129	rBV	33252	41087	5.79%	0.727%
3	1.912	170	178	192	rVB	78530	102181	14.39%	1.809%
4	2.565	368	381	395	rBV	129885	207267	29.19%	3.669%
5	3.186	558	574	589	rBV2	6978	15556	2.19%	0.275%
6	3.838	756	777	798	rVB	7288	22117	3.11%	0.391%
7	4.620	1007	1020	1064	rBV	116429	313218	44.11%	5.544%
8	5.060	1142	1157	1178	rBV2	144228	315213	44.39%	5.579%
9	5.723	1343	1363	1390	rBV3	251092	675948	95.18%	11.965%
10	6.250	1513	1527	1546	rBV	216832	417025	58.72%	7.382%
11	6.690	1650	1664	1684	rBV	181339	352111	49.58%	6.233%
12	7.565	1924	1936	1960	rBV2	69785	124288	17.50%	2.200%
13	7.896	2026	2039	2057	rBV	259602	452865	63.77%	8.016%
14	8.179	2116	2127	2142	rBV	45397	76005	10.70%	1.345%
15	8.636	2256	2269	2310	rBV3	304207	710161	100.00%	12.570%
16	9.417	2498	2512	2533	rBV	355471	592158	83.38%	10.482%
17	10.291	2773	2784	2794	rVB4	14100	23822	3.35%	0.422%
18	10.754	2913	2928	2947	rBV	146672	236612	33.32%	4.188%
19	11.812	3245	3257	3274	rBV	278638	449911	63.35%	7.964%
20	12.063	3323	3335	3350	rBV6	5855	11912	1.68%	0.211%
21	12.192	3363	3375	3395	rBV	253781	413475	58.22%	7.319%




Sum of corrected areas: 5649537

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051290.D
Acq On : 08 Oct 2022 22:38
Operator : JC/MD
Sample : N4931-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

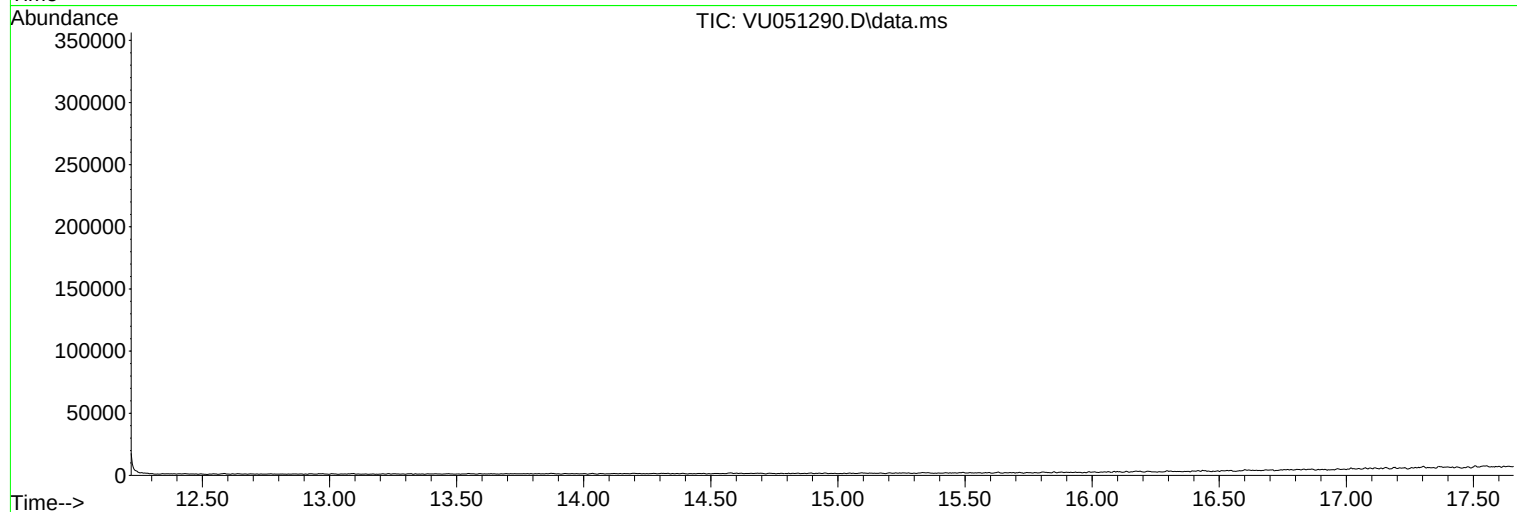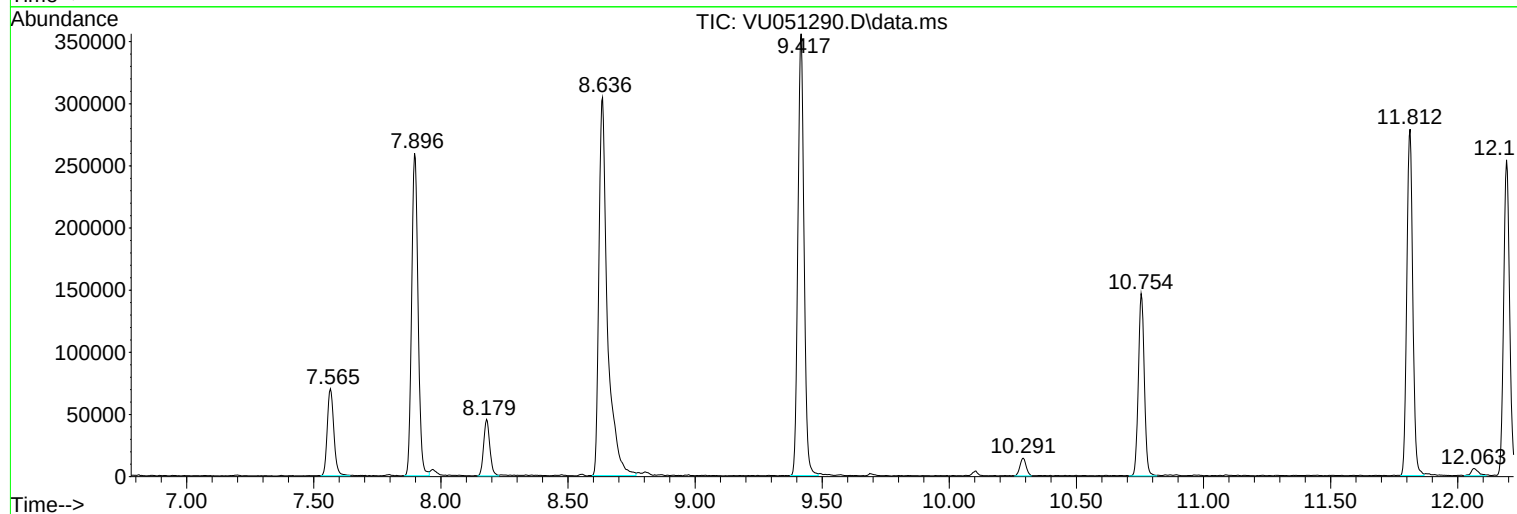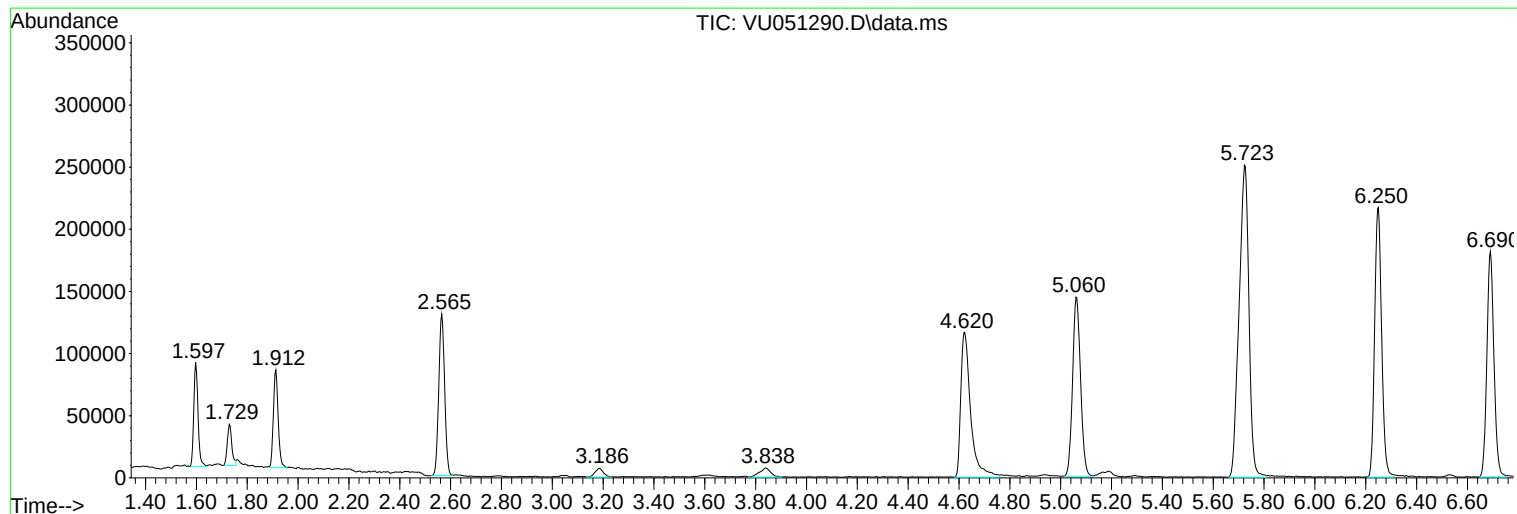

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051290.D
Acq On : 08 Oct 2022 22:38
Operator : JC/MD
Sample : N4931-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
Data File : VU051290.D
Acq On : 08 Oct 2022 22:38
Operator : JC/MD
Sample : N4931-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5H05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc