


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100722\
 Data File : VU051212.D
 Acq On : 07 Oct 2022 11:06
 Operator : JC/MD
 Sample : BFB151
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB151

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Oct 11 02:38:56 2022

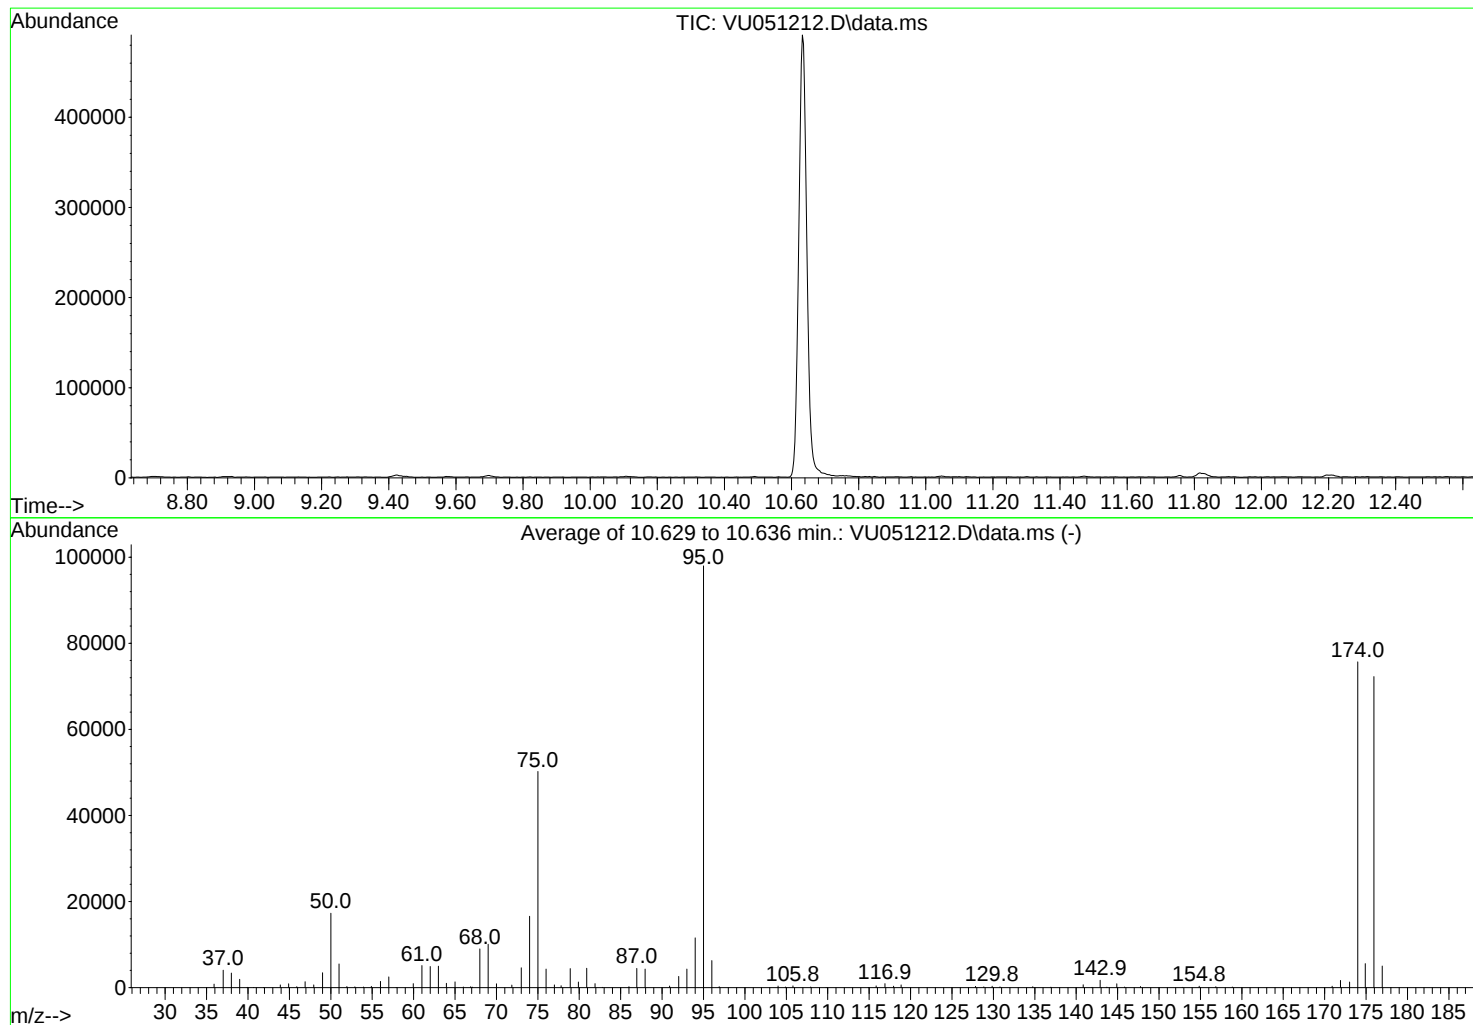

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	17307	PASS
75	95	30	80	51.3	50221	PASS
95	95	100	100	100.0	97989	PASS
96	95	5	9	6.4	6291	PASS
173	174	0.00	2	1.7	1297	PASS
174	95	50	120	77.2	75669	PASS
175	174	5	9	7.4	5586	PASS
176	174	95	101	95.5	72261	PASS
177	176	5	9	7.0	5024	PASS

Scan 2876 (10.587 min): VU051212.D\data.ms
BFB151

m/z	Abundance
40.00	361.0
43.90	446.0

Instrument :
MSVOA_U
ClientSampleId :
BFB151

m/z	Abundance
35.90	865.0
37.00	3963.0
38.00	3407.0
39.00	1947.0
39.90	468.0
43.90	1152.0
44.90	920.0
45.90	201.0
46.90	1349.0
48.00	678.0
49.00	3541.0
50.00	17272.0
51.00	5540.0
51.90	228.0
52.90	155.0
54.00	128.0
54.90	300.0
56.00	1406.0
57.00	2376.0
60.00	980.0
61.00	4689.0
62.00	4735.0
63.00	4370.0
64.00	980.0
65.00	1183.0
66.00	105.0
66.90	376.0
68.00	8627.0
69.00	9781.0
70.00	840.0
71.90	585.0
73.00	4333.0
74.00	16141.0
75.00	48440.0
76.00	4028.0
77.00	537.0
77.80	483.0
78.90	4347.0
79.90	1204.0
80.90	4394.0
81.90	922.0
82.80	125.0
86.00	216.0
86.90	4516.0
87.90	4218.0
90.90	296.0
92.00	2687.0
93.00	4195.0
94.00	11005.0
95.00	94760.0
96.00	6028.0
96.90	197.0
104.00	347.0
104.90	173.0
105.80	364.0
107.90	141.0
115.90	417.0
116.90	924.0
118.00	283.0
118.80	578.0
127.90	319.0
128.90	168.0
129.90	340.0
130.80	186.0
134.80	206.0
137.00	116.0
140.90	631.0
141.90	143.0
142.90	1642.0
144.90	936.0
145.90	134.0
147.70	222.0
154.90	289.0
156.90	221.0
158.90	125.0
170.90	333.0
171.90	1610.0
173.00	1127.0
174.00	71696.0
174.90	5364.0
175.90	68936.0
176.90	4664.0
178.00	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB151

m/z	Abundance
35.90	846.0
37.00	4189.0
38.00	3463.0
39.00	2046.0
39.90	431.0
43.90	1082.0
44.90	933.0
45.90	240.0
46.90	1421.0
47.90	617.0
49.00	3505.0
50.00	17736.0
51.00	5598.0
51.90	249.0
52.90	188.0
54.00	151.0
54.90	329.0
56.00	1480.0
57.00	2574.0
57.90	100.0
59.90	903.0
61.00	5357.0
62.00	5081.0
63.00	5207.0
63.90	1060.0
65.00	1360.0
66.00	170.0
66.90	320.0
68.00	9127.0
69.00	10350.0
70.00	940.0
71.80	600.0
73.00	4755.0
74.00	17168.0
75.00	52016.0
76.00	4439.0
77.00	646.0
77.80	454.0
78.90	4521.0
79.90	1350.0
80.90	4635.0
81.90	980.0
82.80	109.0
86.00	237.0
86.90	4593.0
87.90	4471.0
90.90	378.0
92.00	2609.0
93.00	4411.0
94.00	11980.0
95.00	100736.0
96.00	6402.0
96.90	225.0
104.00	402.0
104.90	157.0
105.80	427.0
107.90	135.0
109.80	102.0
115.80	421.0
116.90	956.0
118.00	363.0
118.90	631.0
127.90	307.0
128.80	180.0
129.90	344.0
130.80	228.0
134.70	225.0
136.90	101.0
140.80	670.0
141.90	128.0
142.90	1794.0
143.70	145.0
144.90	933.0
145.80	144.0
147.70	262.0
152.80	113.0
154.90	335.0
156.90	234.0
158.90	133.0
170.90	328.0
171.90	1736.0
173.00	1321.0
174.00	77816.0
174.90	5758.0
175.90	74400.0
177.00	5225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB151

m/z	Abundance
35.90	757.0
37.00	4037.0
38.00	3270.0
39.00	1873.0
39.90	389.0
40.70	136.0
41.90	108.0
43.90	1016.0
44.90	822.0
45.90	196.0
46.90	1355.0
47.90	618.0
49.00	3328.0
50.00	16912.0
51.00	5346.0
52.00	262.0
52.90	211.0
53.90	132.0
54.90	308.0
56.00	1510.0
57.00	2491.0
59.90	855.0
61.00	5384.0
62.00	4874.0
63.00	5375.0
63.90	1018.0
65.00	1429.0
66.00	219.0
67.10	295.0
68.00	9241.0
69.00	10048.0
70.00	926.0
71.90	582.0
73.00	4711.0
74.00	16384.0
75.00	50208.0
76.00	4500.0
77.00	741.0
77.80	451.0
78.90	4404.0
79.90	1327.0
80.90	4440.0
81.90	914.0
86.00	221.0
87.00	4290.0
88.00	4235.0
90.90	441.0
92.00	2479.0
93.00	4319.0
94.00	11748.0
95.00	98472.0
96.00	6443.0
96.90	203.0
104.00	410.0
104.90	128.0
105.80	429.0
108.00	126.0
114.90	108.0
115.80	357.0
116.90	918.0
117.90	400.0
118.90	680.0
127.80	286.0
128.80	194.0
129.80	356.0
130.80	196.0
134.70	198.0
136.90	118.0
140.90	669.0
142.90	1704.0
143.70	209.0
144.90	823.0
145.80	196.0
147.80	254.0
152.80	109.0
154.80	338.0
156.80	193.0
158.80	153.0
170.90	400.0
171.90	1710.0
173.00	1443.0
174.00	77496.0
174.90	5637.0
176.00	73448.0
177.00	5183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB151