

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
 Data File : VU051372.D
 Acq On : 11 Oct 2022 15:13
 Operator : JC/MD
 Sample : N5026-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BY0

Quant Time: Oct 11 23:37:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 23:36:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	179700	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	206860	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	80556	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	47198	3.256	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	65.200%	
7) Chloroethane-d5	1.909	69	49549	3.978	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	79.600%	
11) 1,1-Dichloroethene-d2	2.565	65	21002	3.665	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	73.400%	
20) 2-Butanone-d5	4.620	46	172404	54.021	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	108.040%	
24) Chloroform-d	5.060	84	135506	5.014	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.200%	
26) 1,2-Dichloroethane-d4	5.700	65	72153	5.177	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.600%	
32) Benzene-d6	5.726	84	231704	4.072	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	81.400%	
36) 1,2-Dichloropropane-d6	6.687	67	87316	4.518	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.400%	
41) Toluene-d8	7.896	98	168185	3.303	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	66.000%#	
43) trans-1,3-Dichloroprop...	8.179	79	25197	3.968	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	79.400%	
46) 2-Hexanone-d5	8.632	63	89211	41.688	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	83.380%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	78085	5.058	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.200%	
66) 1,2-Dichlorobenzene-d4	12.192	152	64971	4.640	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	92.800%	
Target Compounds						
					Qvalue	
13) Acetone	2.626	43	10855	4.535	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051372.D
Acq On : 11 Oct 2022 15:13
Operator : JC/MD
Sample : N5026-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BY0

Quant Time: Oct 11 23:37:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 23:36:07 2022
Response via : Initial Calibration

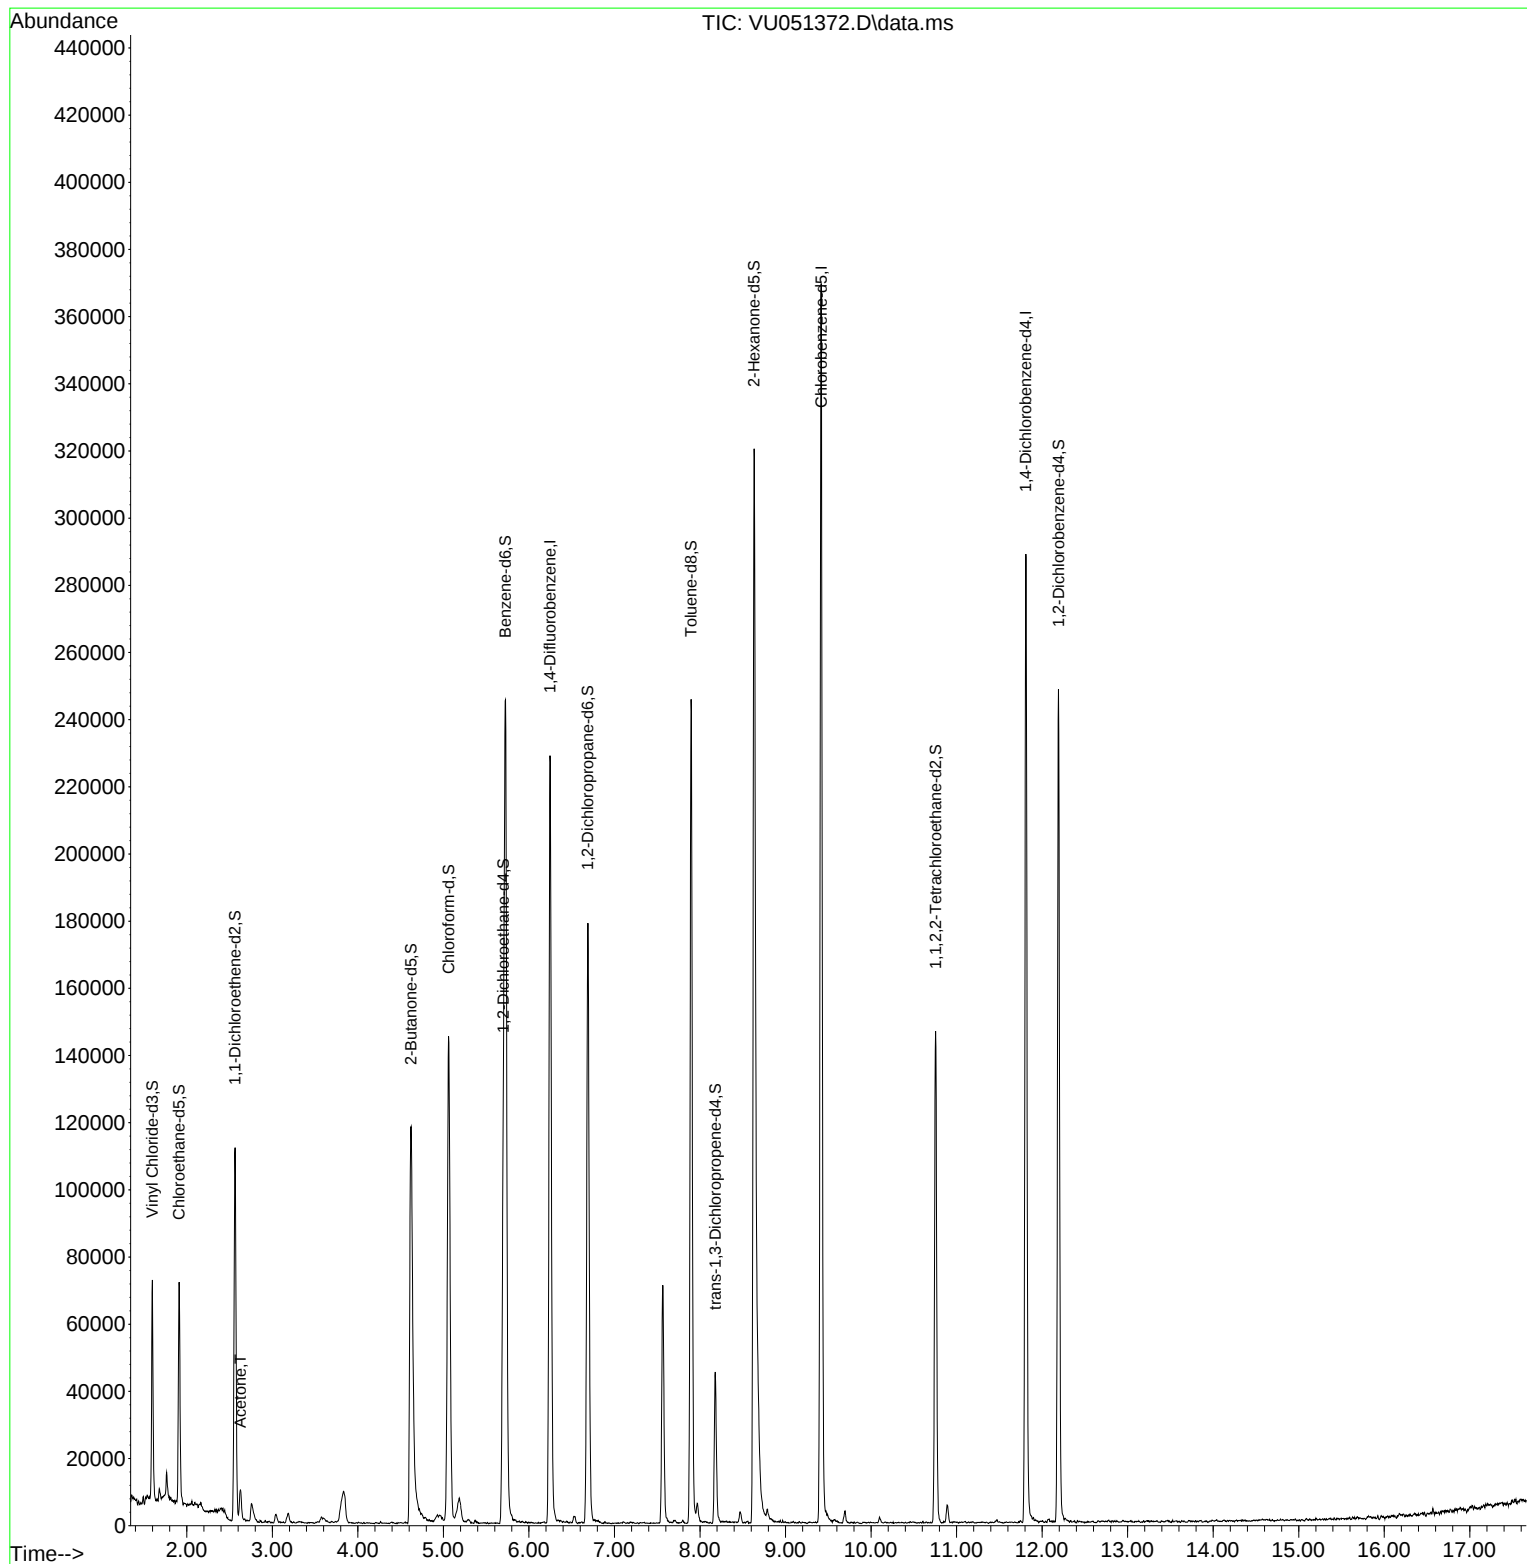

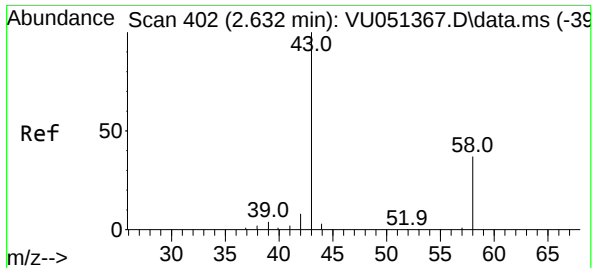

#13
 Acetone
 Concen: 4.535 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. -0.006 min
 Lab File: VU051372.D
 Acq: 11 Oct 2022 15:13

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BY0

Tgt Ion: 43 Resp: 10855
 Ion Ratio Lower Upper
 43 100
 58 33.5 0.0 68.8

