

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
 Data File : VU051379.D
 Acq On : 11 Oct 2022 18:06
 Operator : JC/MD
 Sample : N5072-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BD7

Quant Time: Oct 11 23:39:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 23:36:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	183918	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	217819	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	84050	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	40826	2.752	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	55.000%
7) Chloroethane-d5	1.909	69	44631	3.501	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	70.000%
11) 1,1-Dichloroethene-d2	2.562	65	19331	3.296	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.000%
20) 2-Butanone-d5	4.626	46	199574	61.101	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.200%
24) Chloroform-d	5.060	84	137722	4.979	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%
26) 1,2-Dichloroethane-d4	5.700	65	74881	5.250	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.000%
32) Benzene-d6	5.726	84	224180	3.741	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.800%
36) 1,2-Dichloropropane-d6	6.690	67	88311	4.339	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.800%
41) Toluene-d8	7.896	98	162428	3.030	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	60.600%#
43) trans-1,3-Dichloroprop...	8.179	79	25787	3.857	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.200%
46) 2-Hexanone-d5	8.632	63	110037	48.832	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.660%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	82436	5.071	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.400%
66) 1,2-Dichlorobenzene-d4	12.192	152	70006	4.792	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.800%
Target Compounds						
					Qvalue	
13) Acetone	2.636	43	16426	6.705	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051379.D
Acq On : 11 Oct 2022 18:06
Operator : JC/MD
Sample : N5072-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BD7

Quant Time: Oct 11 23:39:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 23:36:07 2022
Response via : Initial Calibration

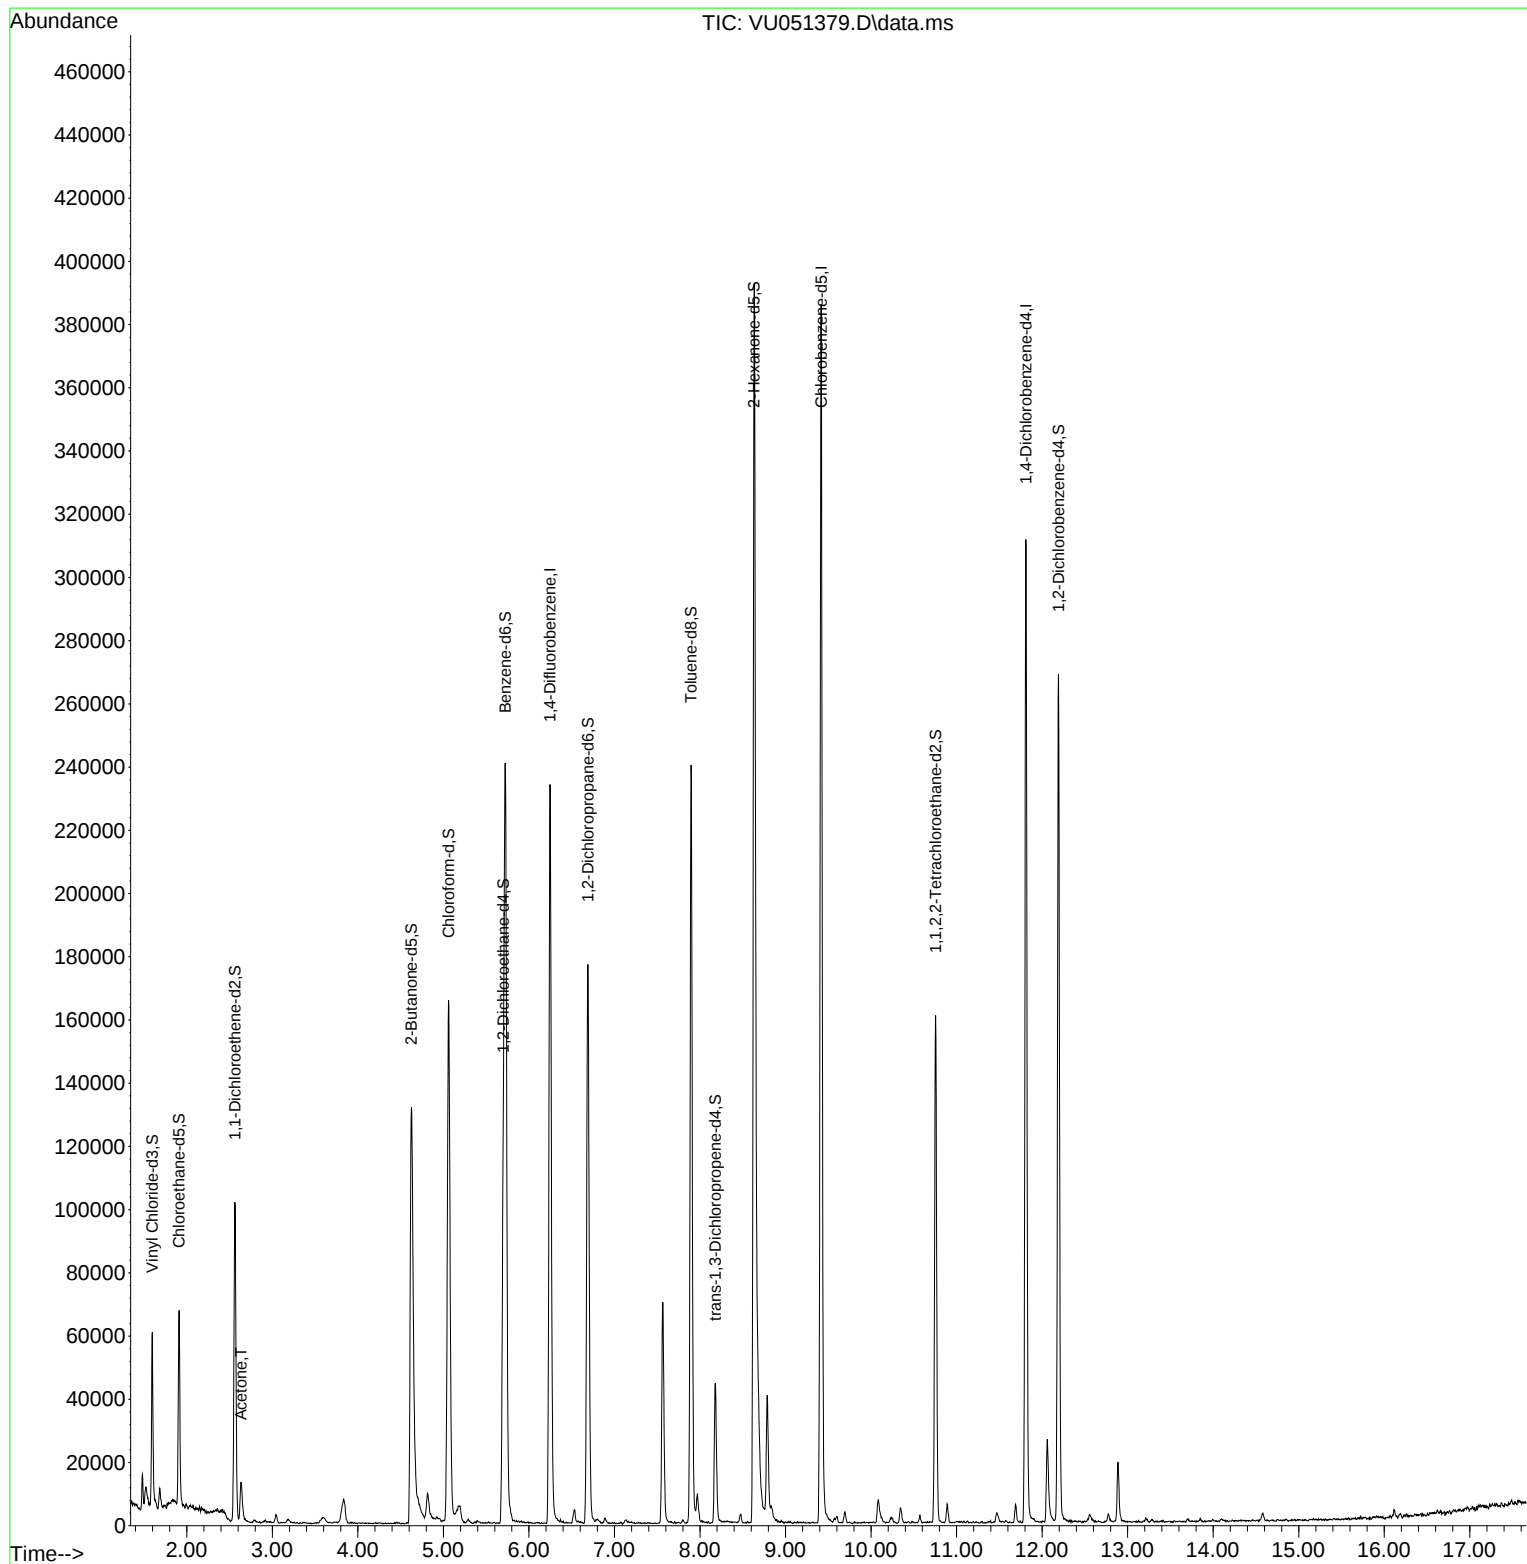

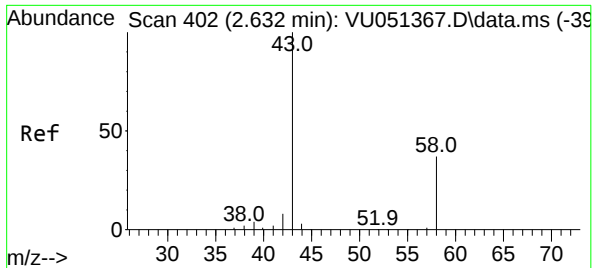

#13
 Acetone
 Concen: 6.705 ug/L
 RT: 2.636 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU051379.D
 Acq: 11 Oct 2022 18:06

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BD7

Tgt Ion: 43 Resp: 16426
 Ion Ratio Lower Upper
 43 100
 58 32.7 0.0 68.8

