

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
 Data File : VU051380.D
 Acq On : 11 Oct 2022 18:31
 Operator : JC/MD
 Sample : N5072-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BG5

Quant Time: Oct 11 23:39:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 23:36:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	184712	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	216672	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	85834	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	39880	2.677	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	53.600%
7) Chloroethane-d5	1.909	69	43390	3.389	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	67.800%
11) 1,1-Dichloroethene-d2	2.562	65	18880	3.206	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.200%
20) 2-Butanone-d5	4.630	46	202708	61.793	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	123.580%
24) Chloroform-d	5.064	84	132809	4.781	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
26) 1,2-Dichloroethane-d4	5.700	65	74320	5.188	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.800%
32) Benzene-d6	5.726	84	221218	3.711	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.200%
36) 1,2-Dichloropropane-d6	6.691	67	86505	4.273	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.400%
41) Toluene-d8	7.896	98	159725	2.995	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	60.000%#
43) trans-1,3-Dichloroprop...	8.179	79	26750	4.022	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.400%
46) 2-Hexanone-d5	8.633	63	111523	49.754	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.500%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	81896	5.064	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	69300	4.645	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.000%
Target Compounds						
					Qvalue	
13) Acetone	2.642	43	21001	8.536	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051380.D
Acq On : 11 Oct 2022 18:31
Operator : JC/MD
Sample : N5072-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BG5

Quant Time: Oct 11 23:39:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 23:36:07 2022
Response via : Initial Calibration

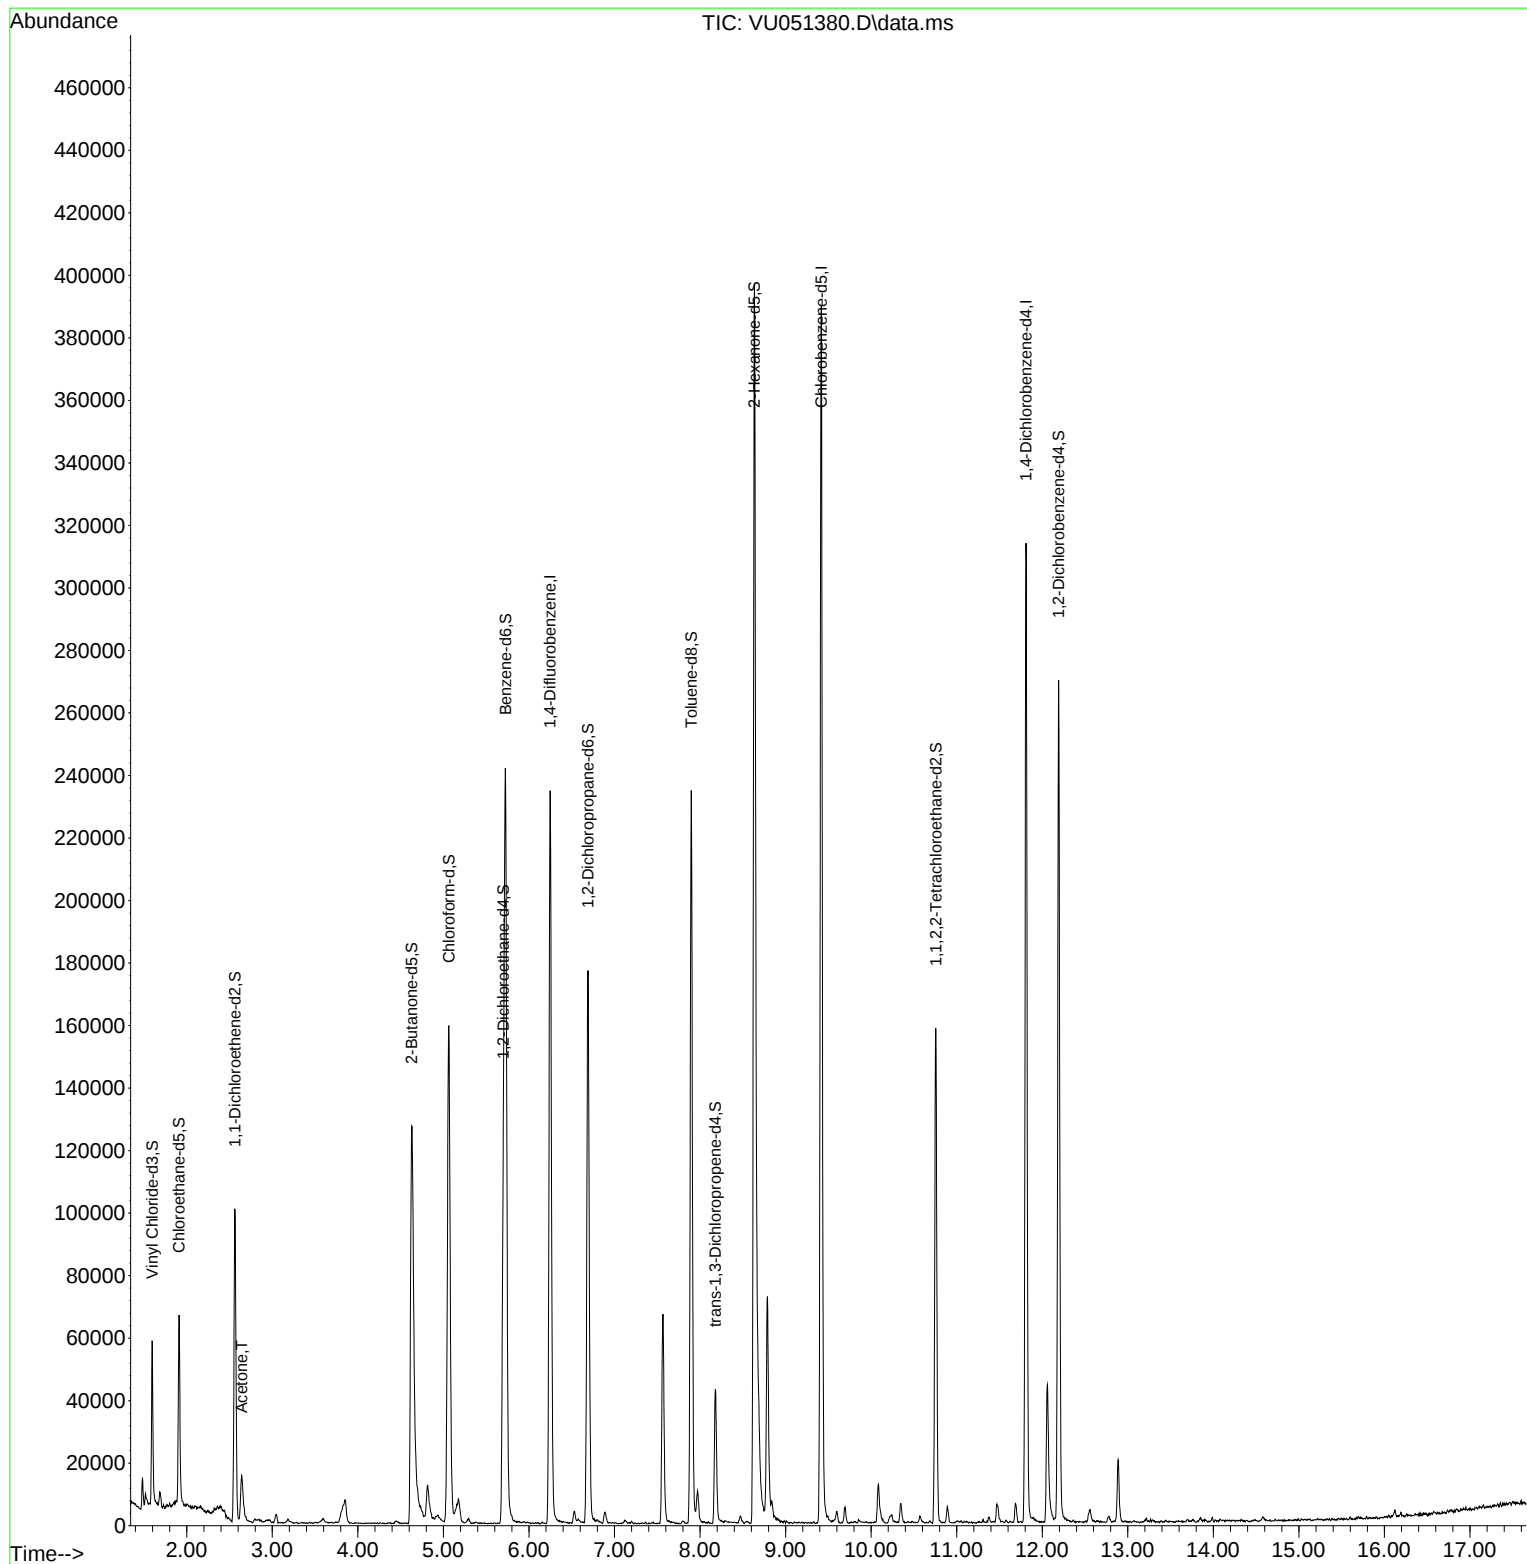

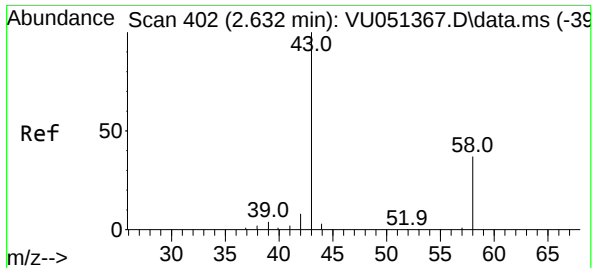

#13
 Acetone
 Concen: 8.536 ug/L
 RT: 2.642 min Scan# 40
 Delta R.T. 0.010 min
 Lab File: VU051380.D
 Acq: 11 Oct 2022 18:31

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BG5

Tgt Ion: 43 Resp: 21001
 Ion Ratio Lower Upper
 43 100
 58 38.0 0.0 68.8

