

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
 Data File : VU051381.D
 Acq On : 11 Oct 2022 18:56
 Operator : JC/MD
 Sample : N5072-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BG8

Quant Time: Oct 11 23:39:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 23:36:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	188171	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	211692	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	80721	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	42051	2.770	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	55.400%
7) Chloroethane-d5	1.909	69	44369	3.402	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	68.000%
11) 1,1-Dichloroethene-d2	2.562	65	20574	3.429	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.600%
20) 2-Butanone-d5	4.639	46	213576	63.910	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	127.820%
24) Chloroform-d	5.063	84	136459	4.822	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%
26) 1,2-Dichloroethane-d4	5.700	65	73837	5.059	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.200%
32) Benzene-d6	5.726	84	221037	3.796	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.000%
36) 1,2-Dichloropropane-d6	6.690	67	88249	4.462	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.200%
41) Toluene-d8	7.896	98	165922	3.185	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	63.600%#
43) trans-1,3-Dichloroprop...	8.179	79	26593	4.093	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.800%
46) 2-Hexanone-d5	8.636	63	118564	54.140	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.280%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	85973	5.442	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.800%
66) 1,2-Dichlorobenzene-d4	12.192	152	69108	4.926	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.600%
Target Compounds					Qvalue	
13) Acetone	2.649	43	25396	10.132	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051381.D
Acq On : 11 Oct 2022 18:56
Operator : JC/MD
Sample : N5072-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BG8

Quant Time: Oct 11 23:39:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 23:36:07 2022
Response via : Initial Calibration

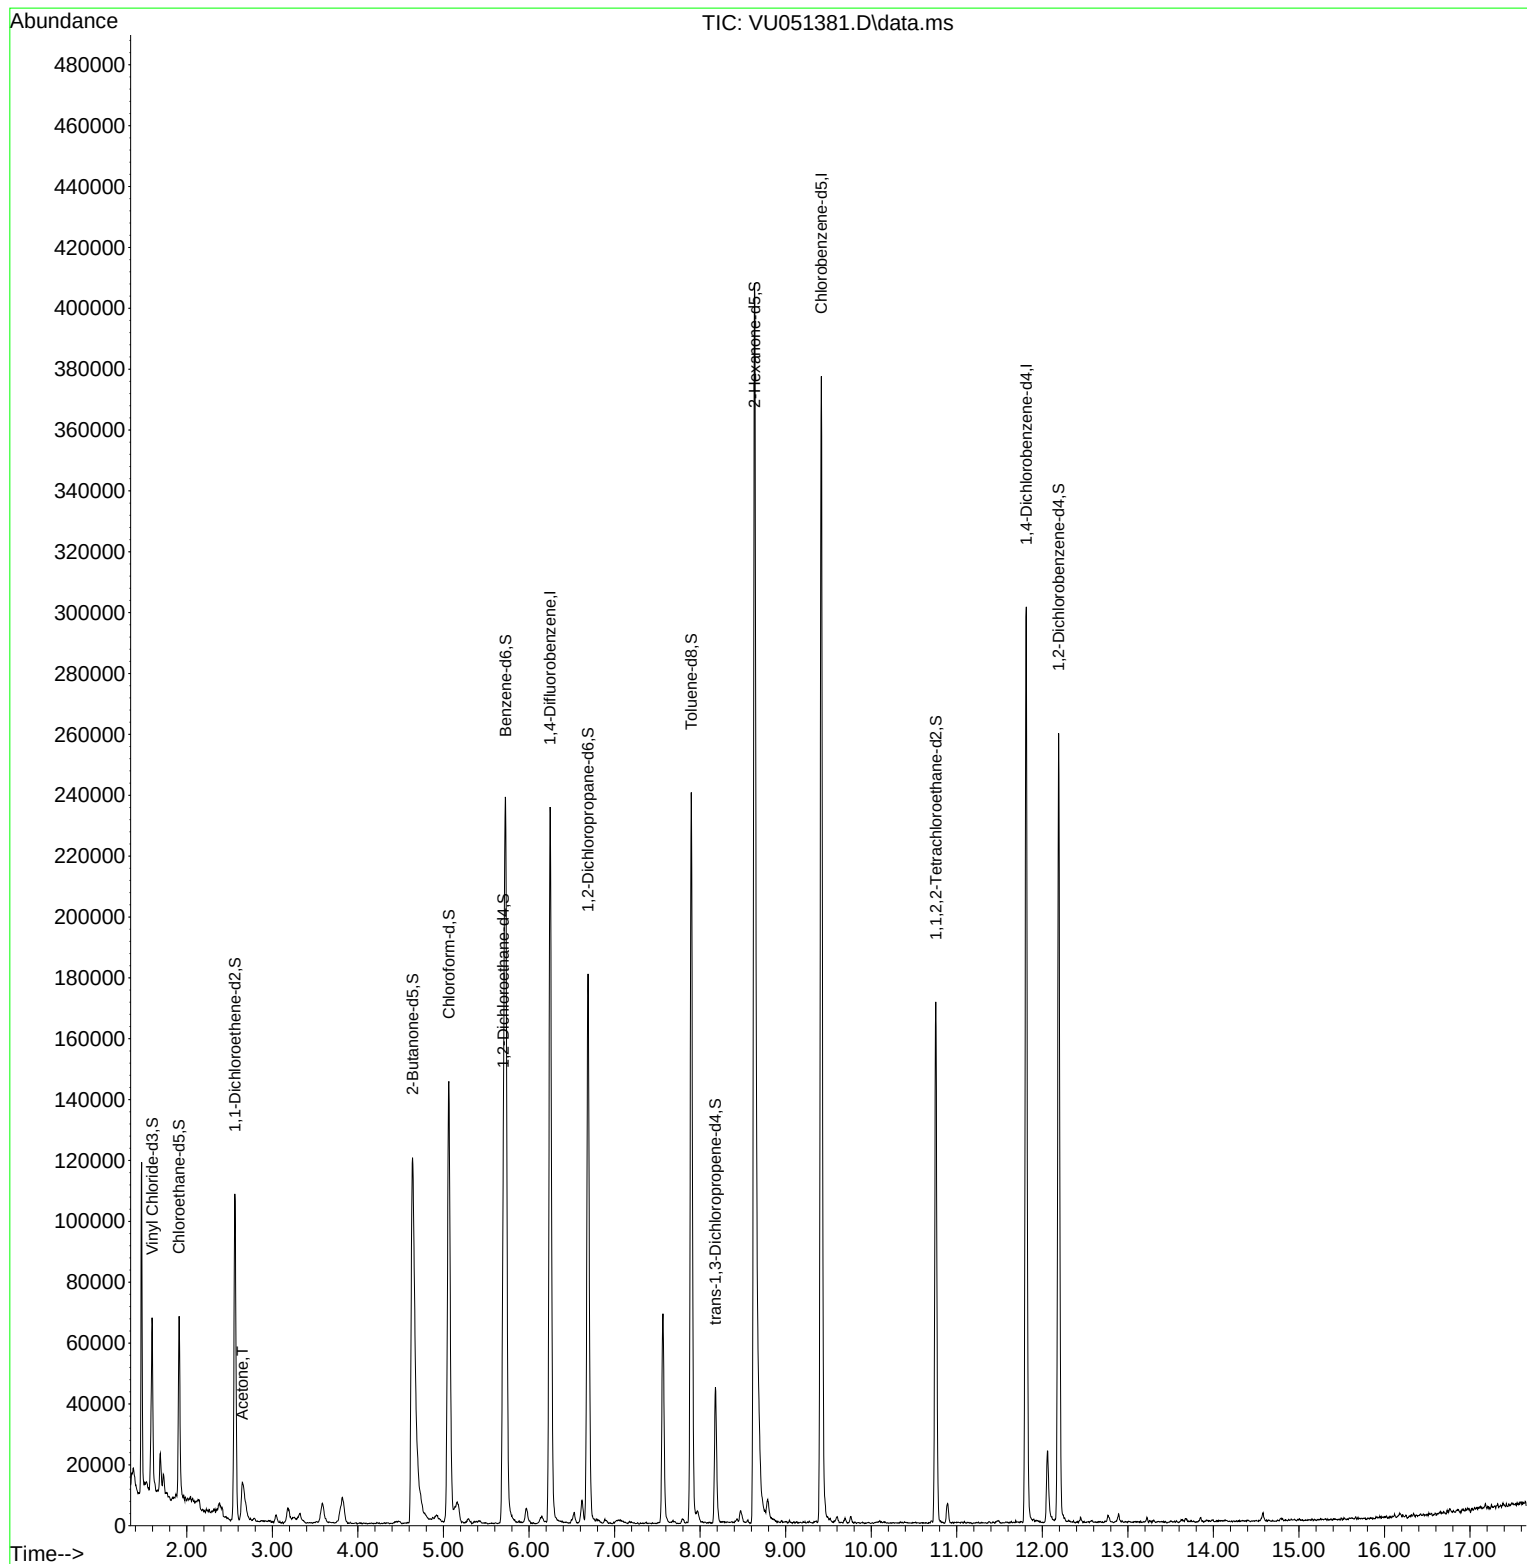

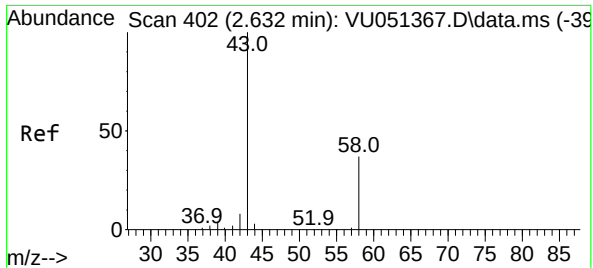

#13
 Acetone
 Concen: 10.132 ug/L
 RT: 2.649 min Scan# 40
 Delta R.T. 0.016 min
 Lab File: VU051381.D
 Acq: 11 Oct 2022 18:56

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BG8

Tgt Ion: 43 Resp: 25396
 Ion Ratio Lower Upper
 43 100
 58 34.3 0.0 68.8

