

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
 Data File : VU051371.D
 Acq On : 11 Oct 2022 14:48
 Operator : JC/MD
 Sample : N5026-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BX7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rVB	66270	74234	10.37%	1.311%
2	1.768	128	133	142	rVB6	8374	9895	1.38%	0.175%
3	1.912	168	178	191	rBV	64603	87713	12.25%	1.549%
4	2.565	369	381	393	rBV	109884	176652	24.68%	3.121%
5	2.626	393	400	416	rVB	9185	15423	2.15%	0.272%
6	2.758	430	441	459	rBV	6145	13064	1.82%	0.231%
7	3.854	762	782	801	rVB	9190	31569	4.41%	0.558%
8	4.620	1005	1020	1041	rBV	122835	303045	42.33%	5.353%
9	5.060	1141	1157	1178	rBV	140800	314730	43.96%	5.560%
10	5.208	1178	1203	1218	rVB	8167	31584	4.41%	0.558%
11	5.723	1338	1363	1390	rBV2	243250	652399	91.13%	11.525%
12	6.247	1513	1526	1543	rBV	239630	460625	64.34%	8.137%
13	6.690	1649	1664	1686	rBV	178869	351127	49.05%	6.203%
14	7.565	1922	1936	1952	rBV	71121	125097	17.47%	2.210%
15	7.896	2026	2039	2056	rBV	244804	429668	60.02%	7.590%
16	8.179	2117	2127	2141	rBV	46580	76496	10.69%	1.351%
17	8.632	2255	2268	2300	rBV3	318098	715900	100.00%	12.646%
18	9.417	2498	2512	2529	rBV	386802	653406	91.27%	11.542%
19	10.755	2913	2928	2948	rVB	147955	240182	33.55%	4.243%
20	11.809	3243	3256	3278	rBV	306591	498014	69.56%	8.797%
21	12.192	3363	3375	3395	rBV	241146	400055	55.88%	7.067%


Sum of corrected areas: 5660878

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051371.D
Acq On : 11 Oct 2022 14:48
Operator : JC/MD
Sample : N5026-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

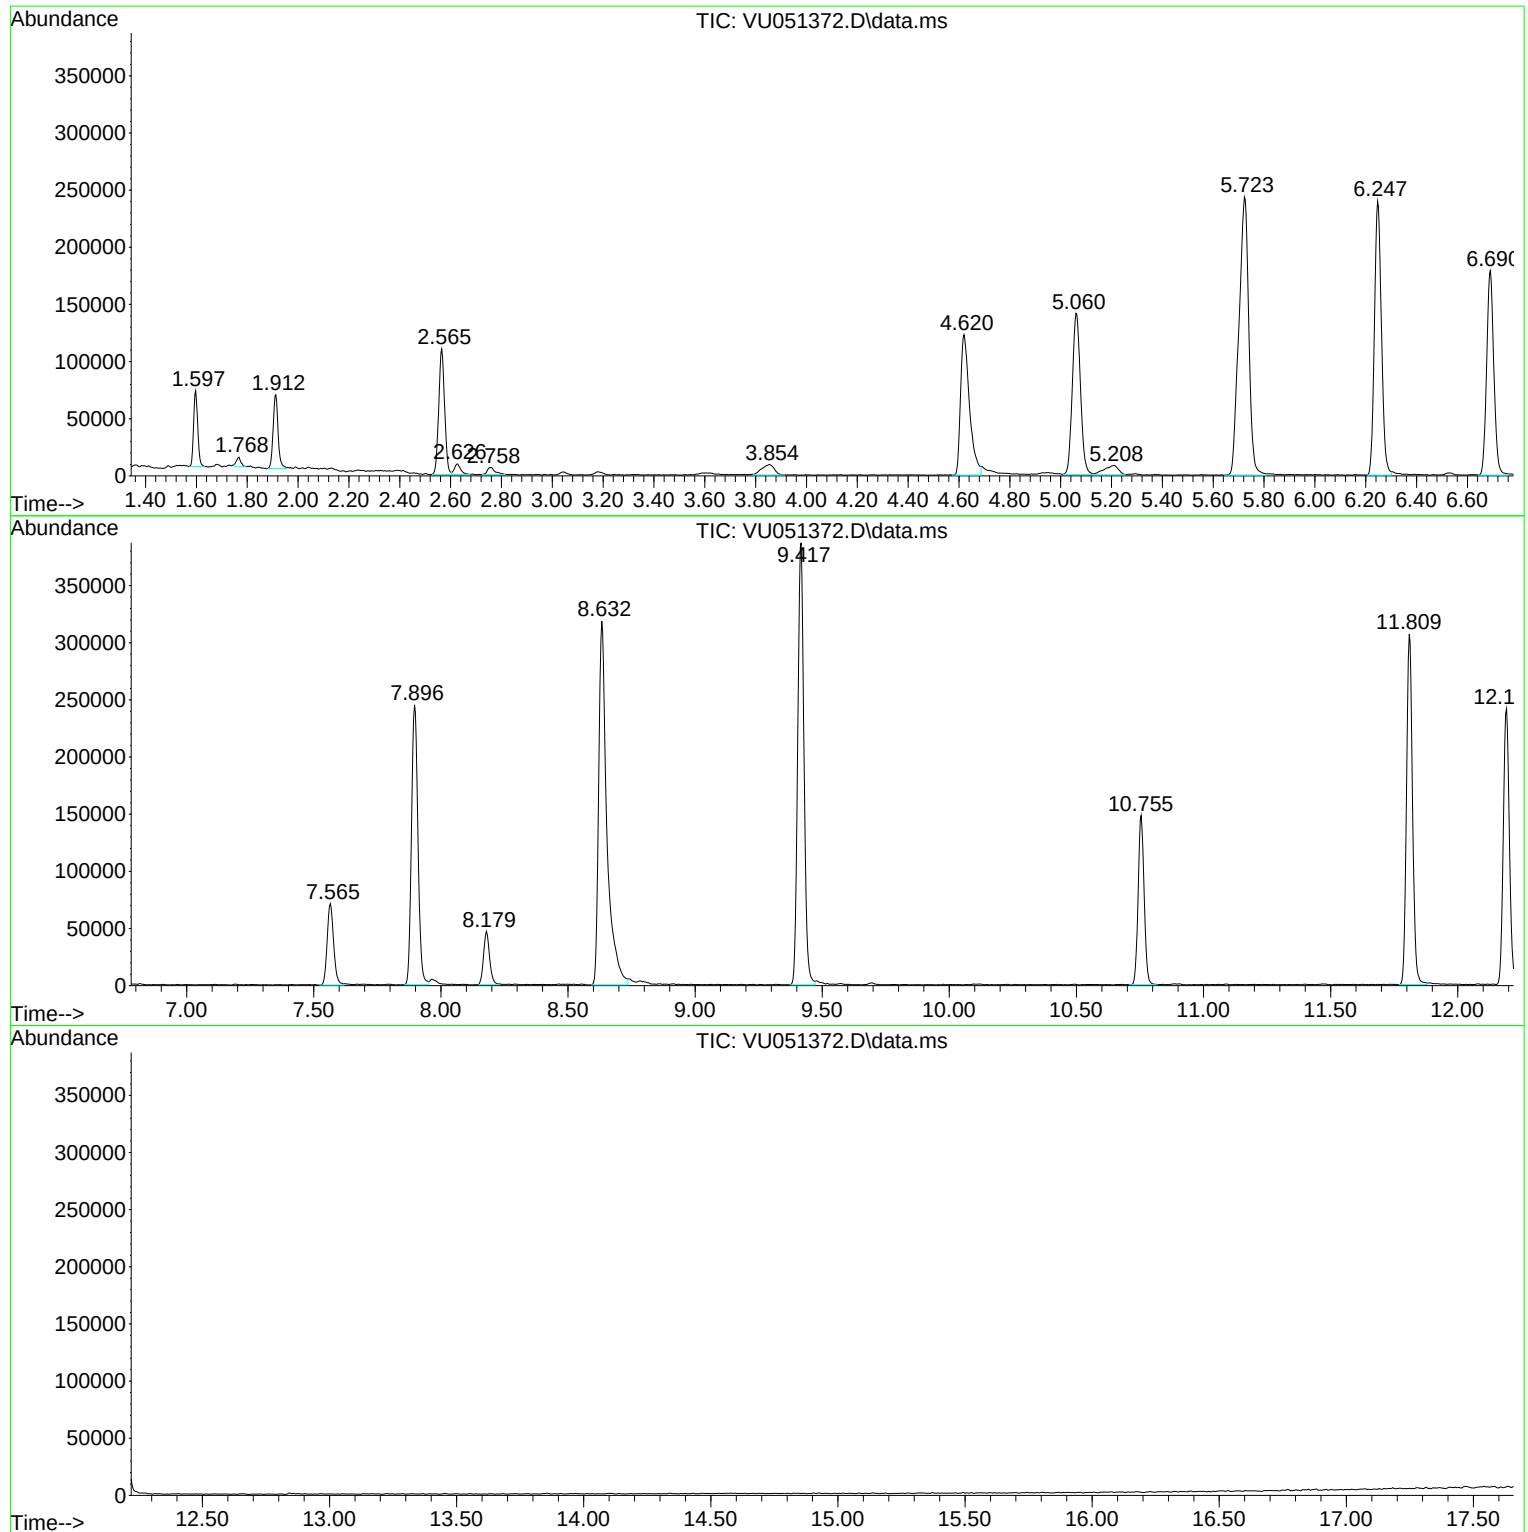

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051371.D
Acq On : 11 Oct 2022 14:48
Operator : JC/MD
Sample : N5026-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051371.D
Acq On : 11 Oct 2022 14:48
Operator : JC/MD
Sample : N5026-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc