

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
 Data File : VU051373.D
 Acq On : 11 Oct 2022 15:38
 Operator : JC/MD
 Sample : N5026-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051374.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	93	rBV	67023	77041	8.39%	1.221%
2	1.765	125	132	140	rBV6	6570	9733	1.06%	0.154%
3	1.909	168	177	200	rVB	72052	98844	10.76%	1.567%
4	2.565	369	381	397	rBV	116944	191105	20.81%	3.029%
5	3.041	518	529	545	rBV	28970	52597	5.73%	0.834%
6	3.183	561	573	586	rBV2	6998	15346	1.67%	0.243%
7	3.835	752	776	794	rVB	5504	18948	2.06%	0.300%
8	4.620	1005	1020	1044	rBV	156065	393613	42.86%	6.239%
9	5.060	1142	1157	1177	rBV	155401	349307	38.04%	5.537%
10	5.176	1179	1193	1207	rVB	5610	16090	1.75%	0.255%
11	5.723	1343	1363	1385	rBV2	268305	726266	79.09%	11.512%
12	6.247	1513	1526	1553	rBV	238169	460170	50.11%	7.294%
13	6.690	1650	1664	1685	rBV	192283	383803	41.79%	6.084%
14	7.565	1924	1936	1955	rBV	79809	138660	15.10%	2.198%
15	7.896	2026	2039	2058	rBV	273036	471825	51.38%	7.479%
16	8.179	2116	2127	2151	rBV2	50478	87276	9.50%	1.383%
17	8.632	2253	2268	2304	rBV2	412545	918299	100.00%	14.556%
18	9.417	2495	2512	2533	rBV	390061	661298	72.01%	10.482%
19	10.755	2915	2928	2943	rBV	172712	280189	30.51%	4.441%
20	11.809	3244	3256	3277	rBV	305292	500503	54.50%	7.933%
21	12.192	3362	3375	3396	rBV	272608	458003	49.88%	7.260%




Sum of corrected areas: 6308916

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU0101122\
Data File : VU051373.D
Acq On : 11 Oct 2022 15:38
Operator : JC/MD
Sample : N5026-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

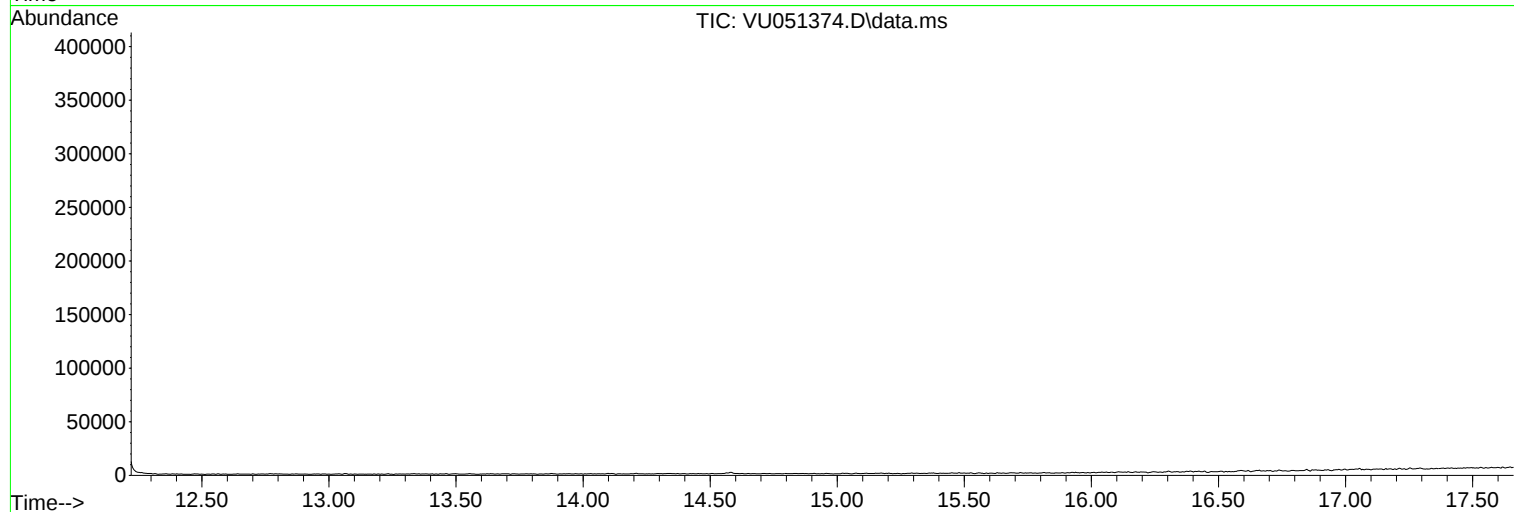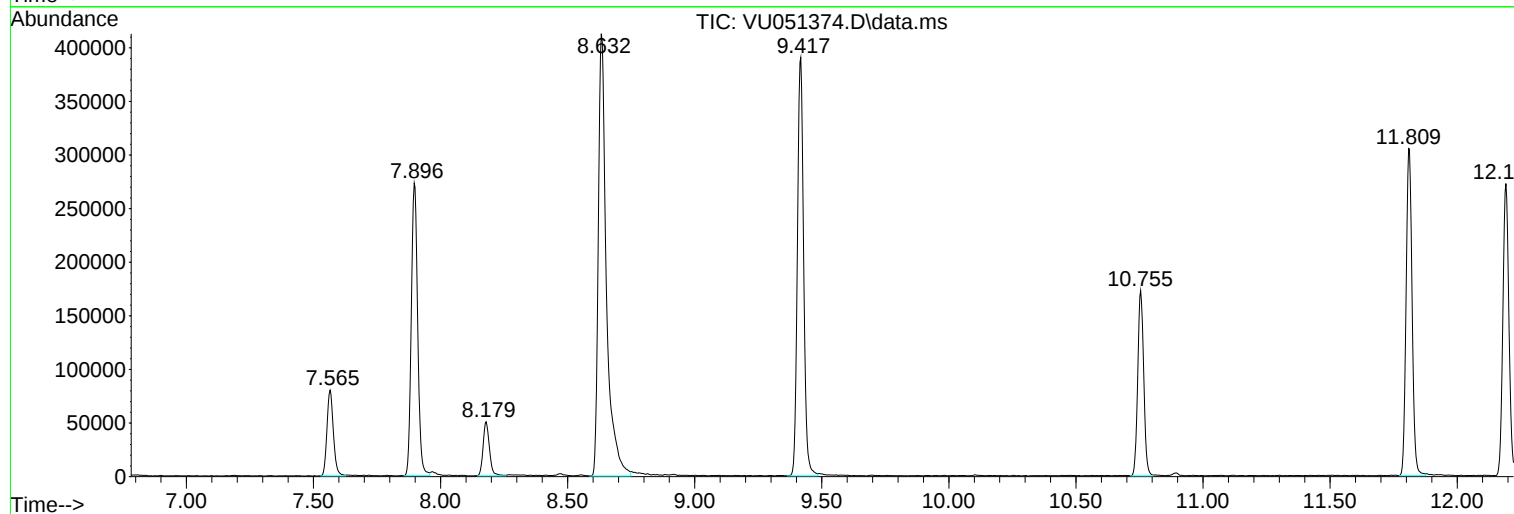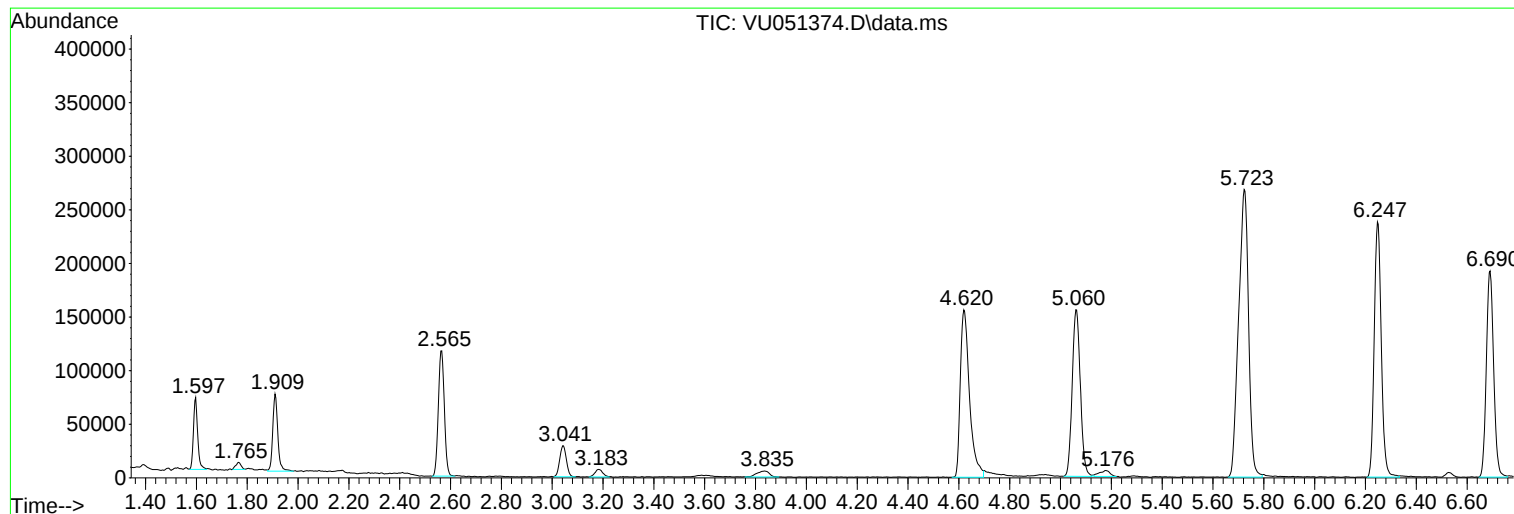

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051373.D
Acq On : 11 Oct 2022 15:38
Operator : JC/MD
Sample : N5026-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051373.D
Acq On : 11 Oct 2022 15:38
Operator : JC/MD
Sample : N5026-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc