

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
 Data File : VU051382.D
 Acq On : 11 Oct 2022 19:21
 Operator : JC/MD
 Sample : N5072-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	96	rVB	68306	79186	8.42%	1.223%
2	1.764	125	132	141	rBV4	6341	10347	1.10%	0.160%
3	1.909	170	177	191	rVB	73420	93228	9.91%	1.439%
4	2.562	368	380	396	rBV	123470	200838	21.36%	3.101%
5	3.044	517	530	547	rVB2	30760	57883	6.16%	0.894%
6	3.182	559	573	590	rVB2	6781	15687	1.67%	0.242%
7	3.848	761	780	794	rVB	4348	12611	1.34%	0.195%
8	4.620	1007	1020	1052	rBV2	159870	405781	43.15%	6.265%
9	5.060	1142	1157	1176	rBV	162267	356878	37.95%	5.510%
10	5.722	1343	1363	1387	rBV2	276937	747222	79.46%	11.536%
11	6.247	1512	1526	1554	rBV	251150	481674	51.22%	7.437%
12	6.690	1650	1664	1683	rBV	201719	396880	42.20%	6.127%
13	7.565	1924	1936	1958	rBV2	78976	139472	14.83%	2.153%
14	7.896	2022	2039	2055	rBV	284636	494602	52.60%	7.636%
15	8.179	2116	2127	2147	rBV	51200	85579	9.10%	1.321%
16	8.632	2252	2268	2311	rBV2	419817	940384	100.00%	14.519%
17	9.417	2498	2512	2534	rBV	405366	683198	72.65%	10.548%
18	10.754	2916	2928	2948	rBV	176024	287373	30.56%	4.437%
19	11.812	3244	3257	3279	rBV	312084	513205	54.57%	7.923%
20	12.192	3363	3375	3390	rBV	281682	462247	49.16%	7.137%
21	16.764	4790	4797	4804	rBV7	9007	12851	1.37%	0.198%




Sum of corrected areas: 6477126

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051382.D
Acq On : 11 Oct 2022 19:21
Operator : JC/MD
Sample : N5072-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

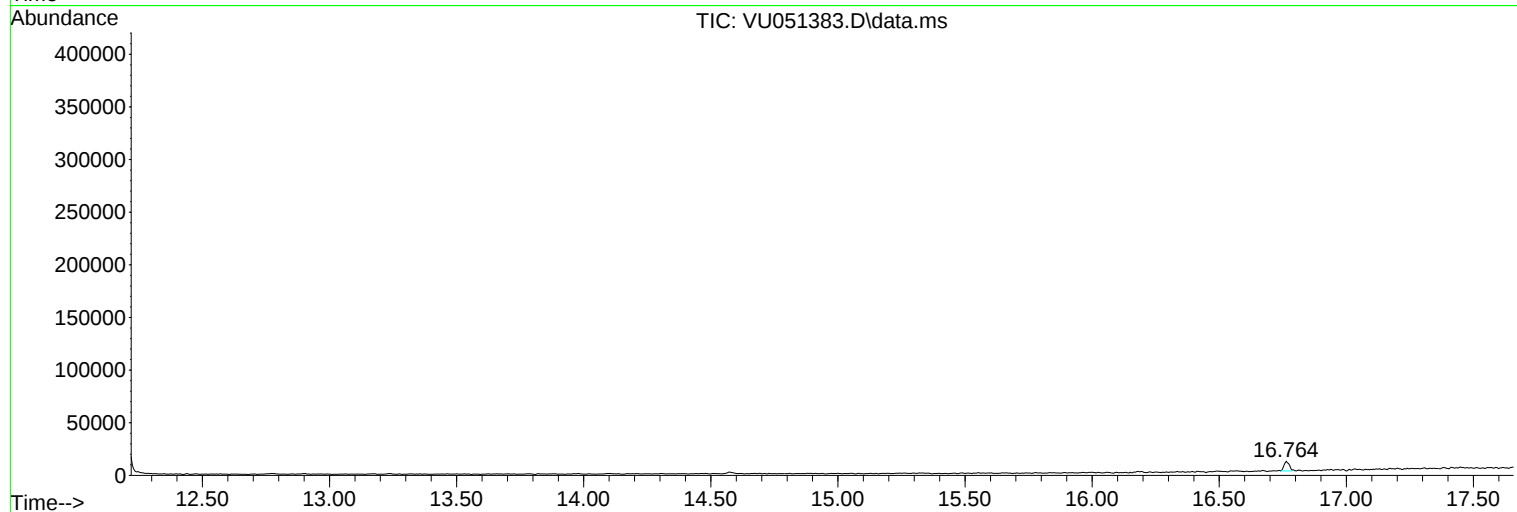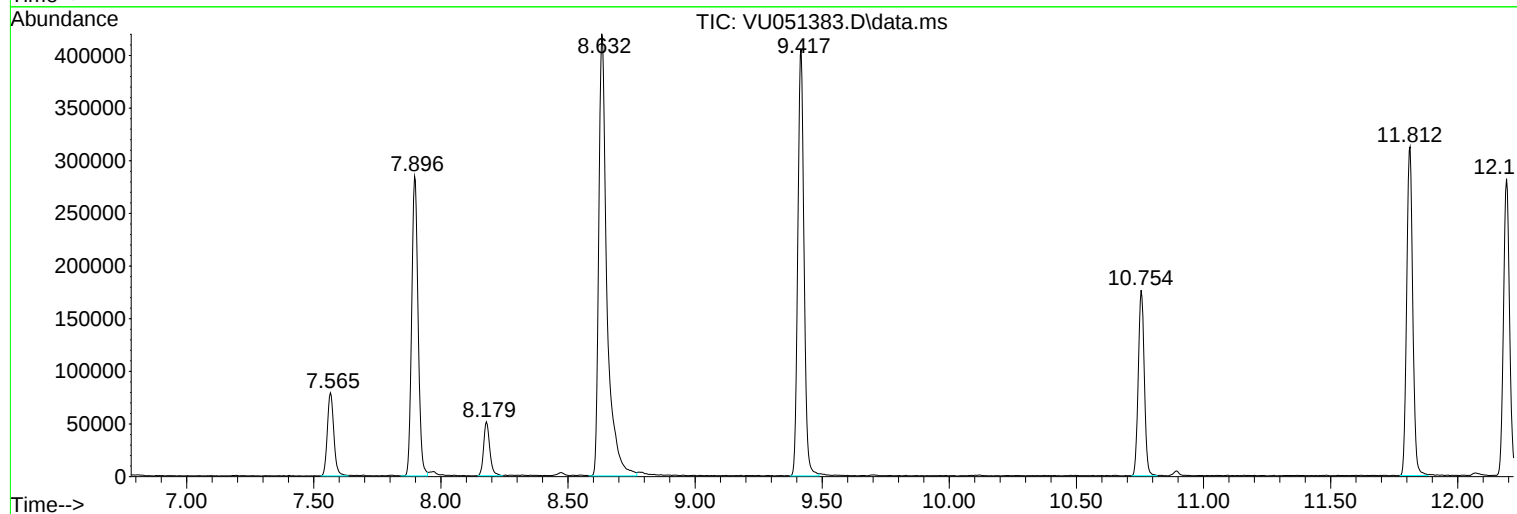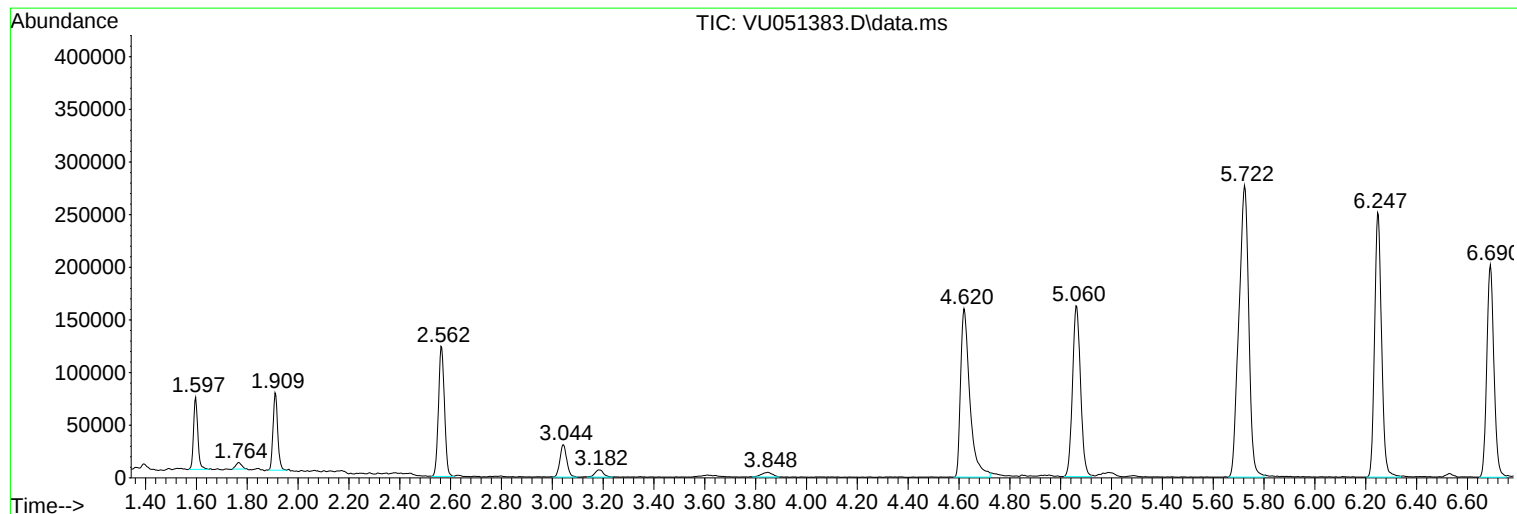

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051382.D
Acq On : 11 Oct 2022 19:21
Operator : JC/MD
Sample : N5072-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051382.D
Acq On : 11 Oct 2022 19:21
Operator : JC/MD
Sample : N5072-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc