

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
 Data File : VU051383.D
 Acq On : 11 Oct 2022 19:45
 Operator : JC/MD
 Sample : VIBLK114
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK114

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	62555	71666	8.07%	1.159%
2	1.764	128	132	142	rVB7	6627	9007	1.01%	0.146%
3	1.909	169	177	190	rBV	67256	89440	10.07%	1.446%
4	2.565	369	381	397	rBV	114841	188682	21.25%	3.051%
5	3.044	519	530	542	rBV2	22005	41075	4.63%	0.664%
6	3.186	554	574	590	rBV	9634	20857	2.35%	0.337%
7	4.620	1008	1020	1062	rBV	151495	400548	45.11%	6.477%
8	5.063	1141	1158	1178	rBV	150781	337566	38.02%	5.459%
9	5.722	1336	1363	1385	rBV2	254786	692431	77.98%	11.198%
10	6.247	1512	1526	1546	rBV	252952	484542	54.57%	7.836%
11	6.690	1646	1664	1691	rBV	188583	376775	42.43%	6.093%
12	7.565	1924	1936	1957	rBV2	73864	132041	14.87%	2.135%
13	7.896	2026	2039	2056	rBV	254923	451189	50.81%	7.296%
14	8.179	2116	2127	2145	rBV2	47287	81830	9.22%	1.323%
15	8.632	2256	2268	2305	rBV4	399248	887953	100.00%	14.360%
16	9.417	2499	2512	2543	rBV	408173	686046	77.26%	11.094%
17	10.754	2915	2928	2945	rBV2	168428	274894	30.96%	4.445%
18	11.809	3245	3256	3273	rBV	316918	516504	58.17%	8.353%
19	12.192	3362	3375	3398	rBV	267146	440649	49.63%	7.126%




Sum of corrected areas: 6183695

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU0101122\
Data File : VU051383.D
Acq On : 11 Oct 2022 19:45
Operator : JC/MD
Sample : VIBLK114
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

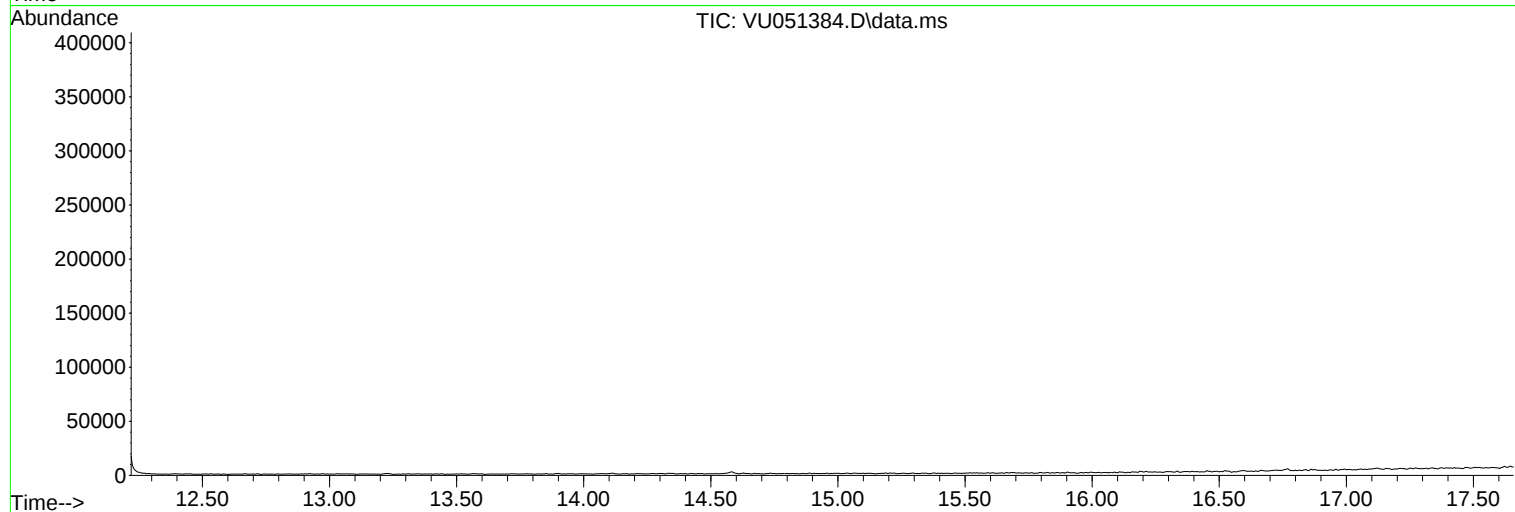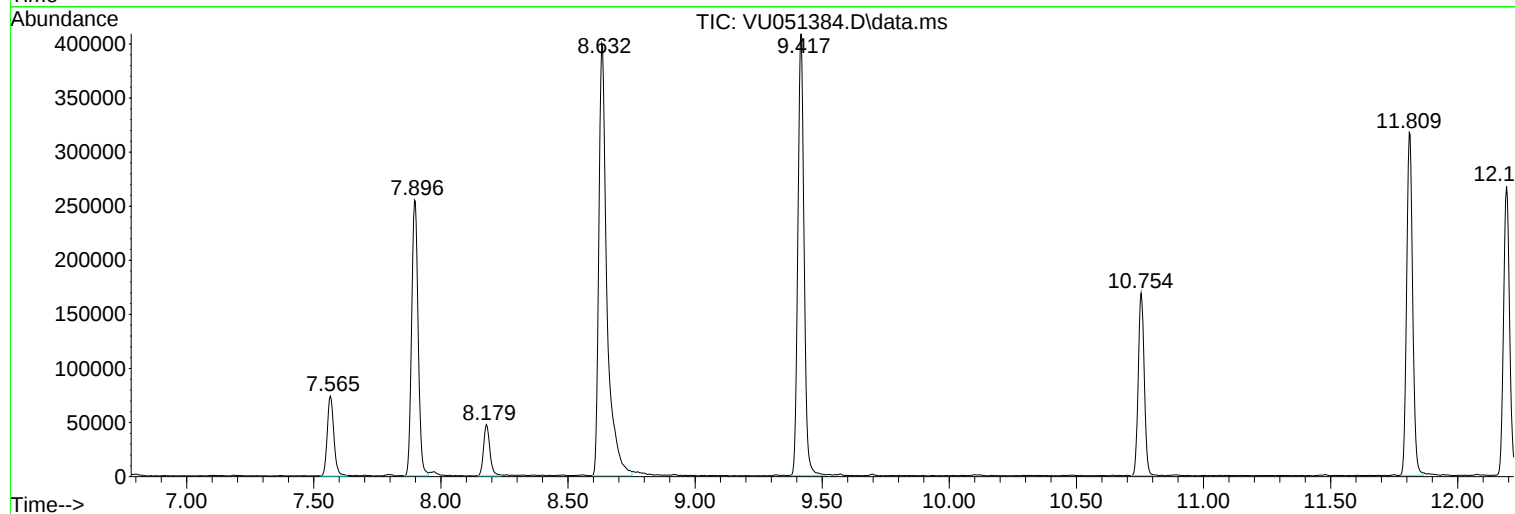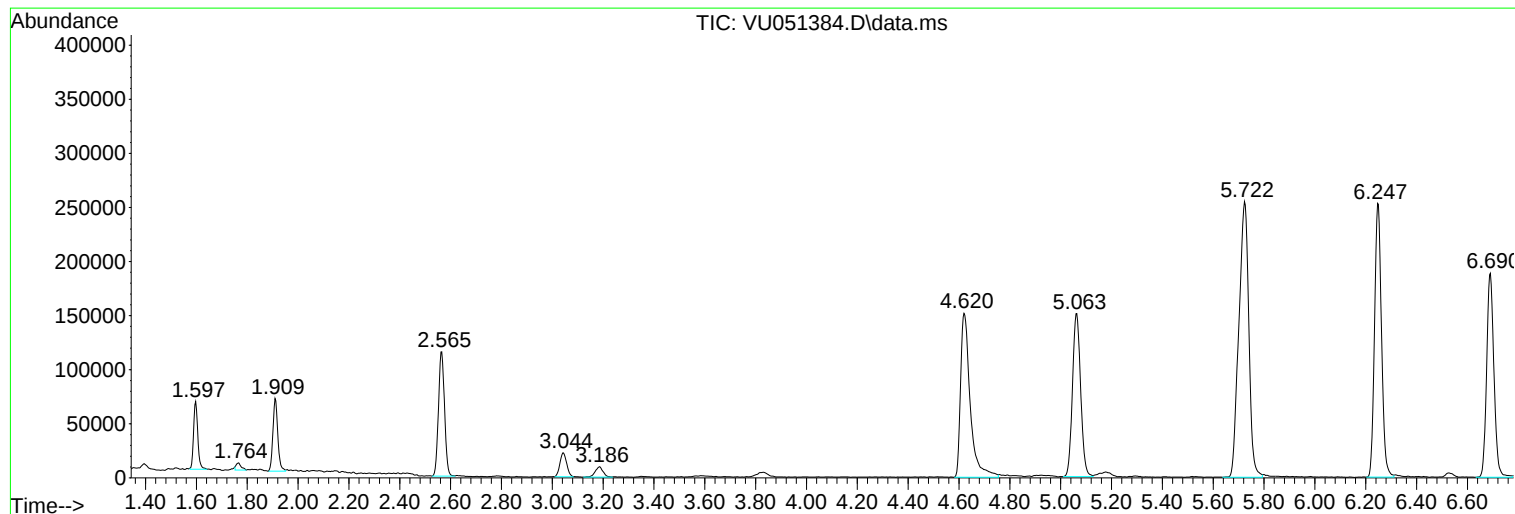

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051383.D
Acq On : 11 Oct 2022 19:45
Operator : JC/MD
Sample : VIBLK114
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101122\
Data File : VU051383.D
Acq On : 11 Oct 2022 19:45
Operator : JC/MD
Sample : VIBLK114
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc