

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110222\
 Data File : VU051682.D
 Acq On : 02 Nov 2022 11:00
 Operator : JC/MD
 Sample : VU1102WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK128

Quant Time: Nov 03 01:46:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 03 01:45:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	162880	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	172731	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	68933	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	69169	5.638	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	112.800%	
7) Chloroethane-d5	1.912	69	62786	4.907	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	98.200%	
11) 1,1-Dichloroethene-d2	2.565	65	27013	6.067	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	121.400%	
20) 2-Butanone-d5	4.639	46	170450	38.366	ug/L	0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	76.740%	
24) Chloroform-d	5.060	84	140479	4.894	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.800%	
26) 1,2-Dichloroethane-d4	5.703	65	71241	4.594	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.800%	
32) Benzene-d6	5.726	84	270511	4.963	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.200%	
36) 1,2-Dichloropropane-d6	6.690	67	91478	4.799	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.000%	
41) Toluene-d8	7.896	98	209153	4.879	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.600%	
43) trans-1,3-Dichloroprop...	8.179	79	28066	4.816	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	96.400%	
46) 2-Hexanone-d5	8.636	63	122960	35.048	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	70.100%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	75740	4.336	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	86.800%	
66) 1,2-Dichlorobenzene-d4	12.192	152	72333	5.717	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	114.400%	
Target Compounds						Qvalue
16) Methylene chloride	3.047	84	5505	0.237	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110222\
Data File : VU051682.D
Acq On : 02 Nov 2022 11:00
Operator : JC/MD
Sample : VU1102WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK128

Quant Time: Nov 03 01:46:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 03 01:45:18 2022
Response via : Initial Calibration

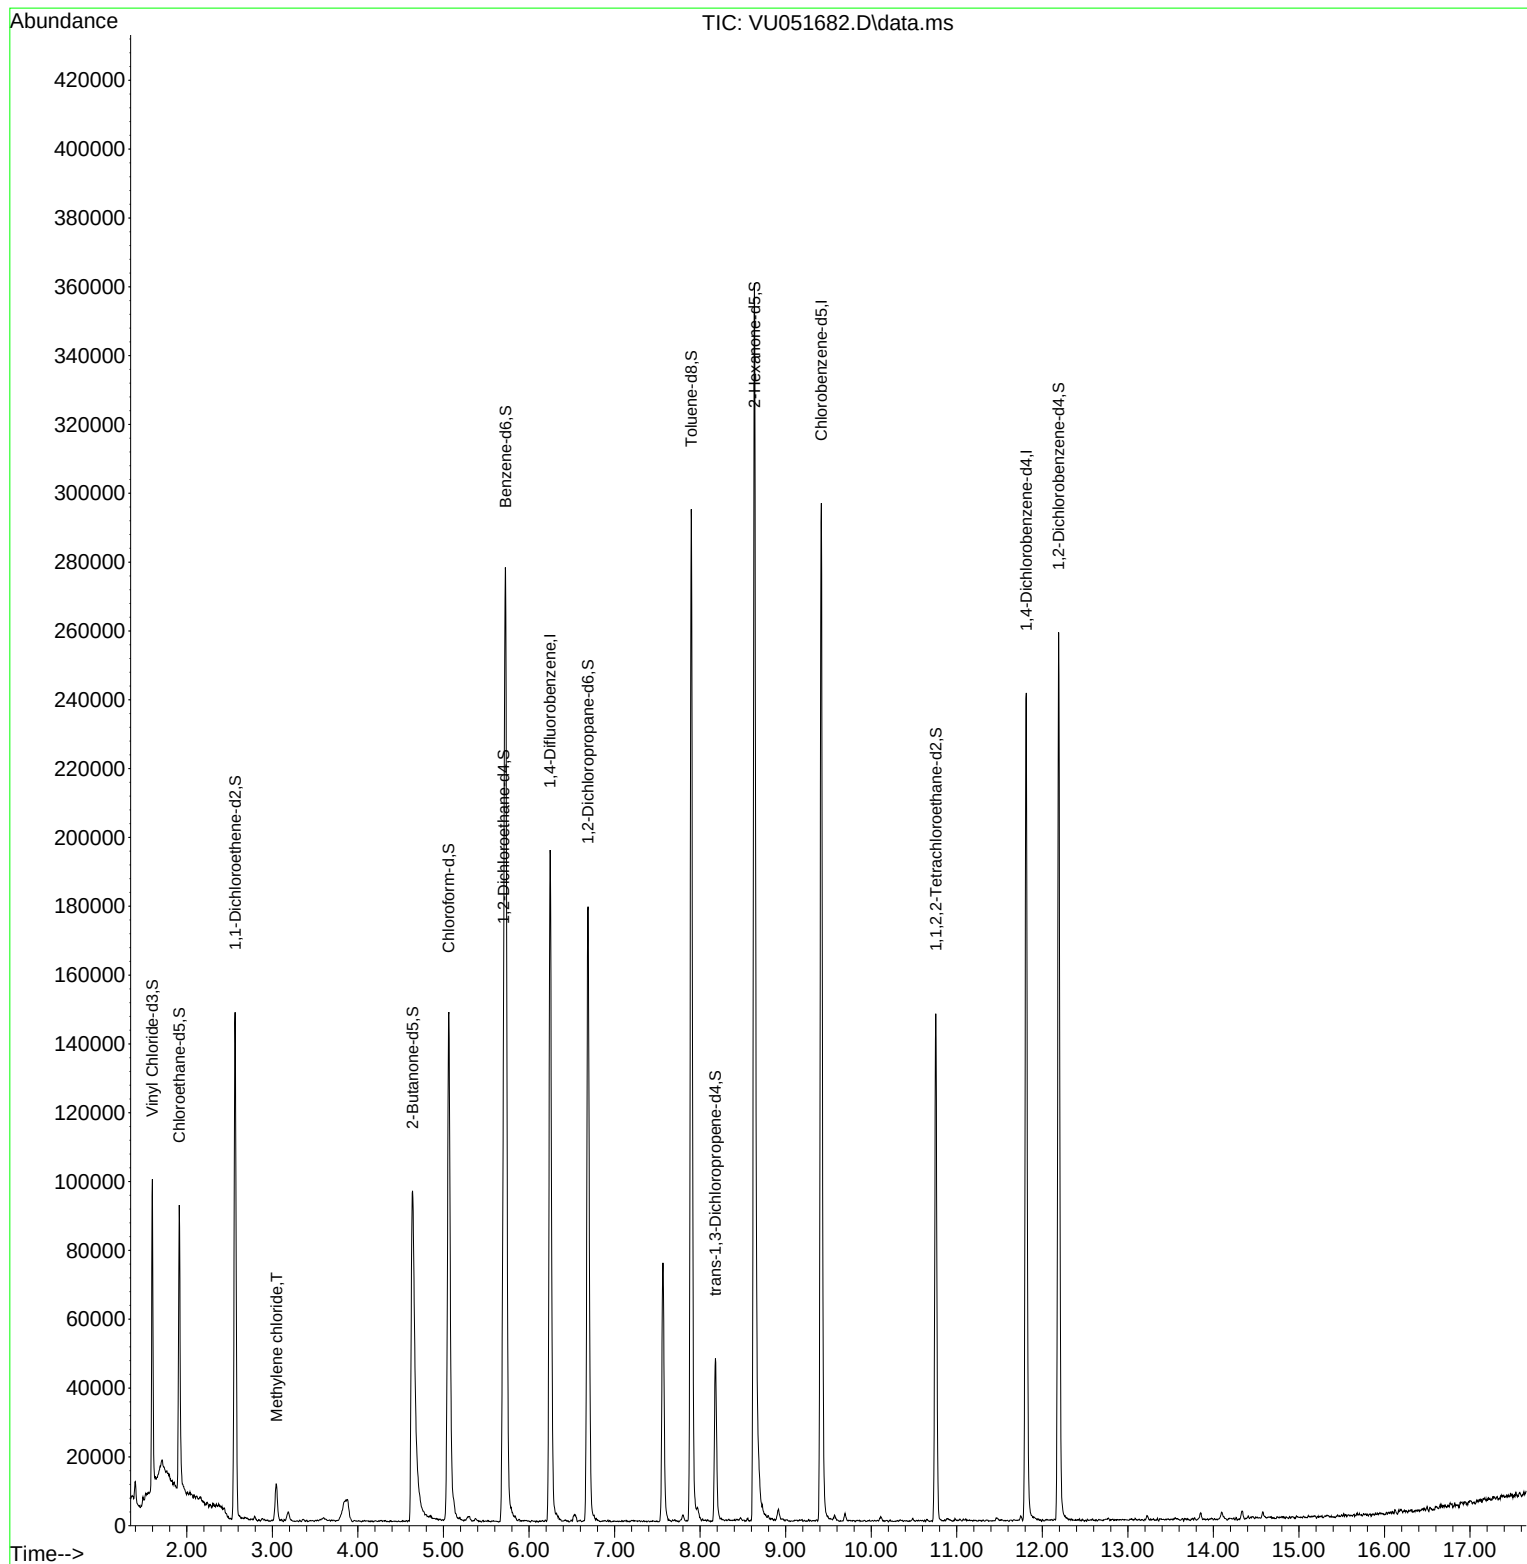

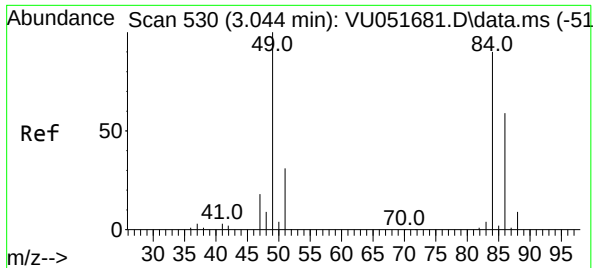

#16
Methylene chloride
Concen: 0.237 ug/L
RT: 3.047 min Scan# 51
Delta R.T. 0.003 min
Lab File: VU051682.D
Acq: 02 Nov 2022 11:00

Instrument :
MSVOA_U
ClientSampleId :
VBLK128

Tgt Ion:	84	Resp:	5505
Ion	Ratio	Lower	Upper
84	100		
86	69.8	46.3	85.9
49	113.8	76.0	141.2

