


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110222\
 Data File : VU051680.D
 Acq On : 02 Nov 2022 08:56
 Operator : JC/MD
 Sample : BFB162
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB162

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Nov 04 00:49:19 2022

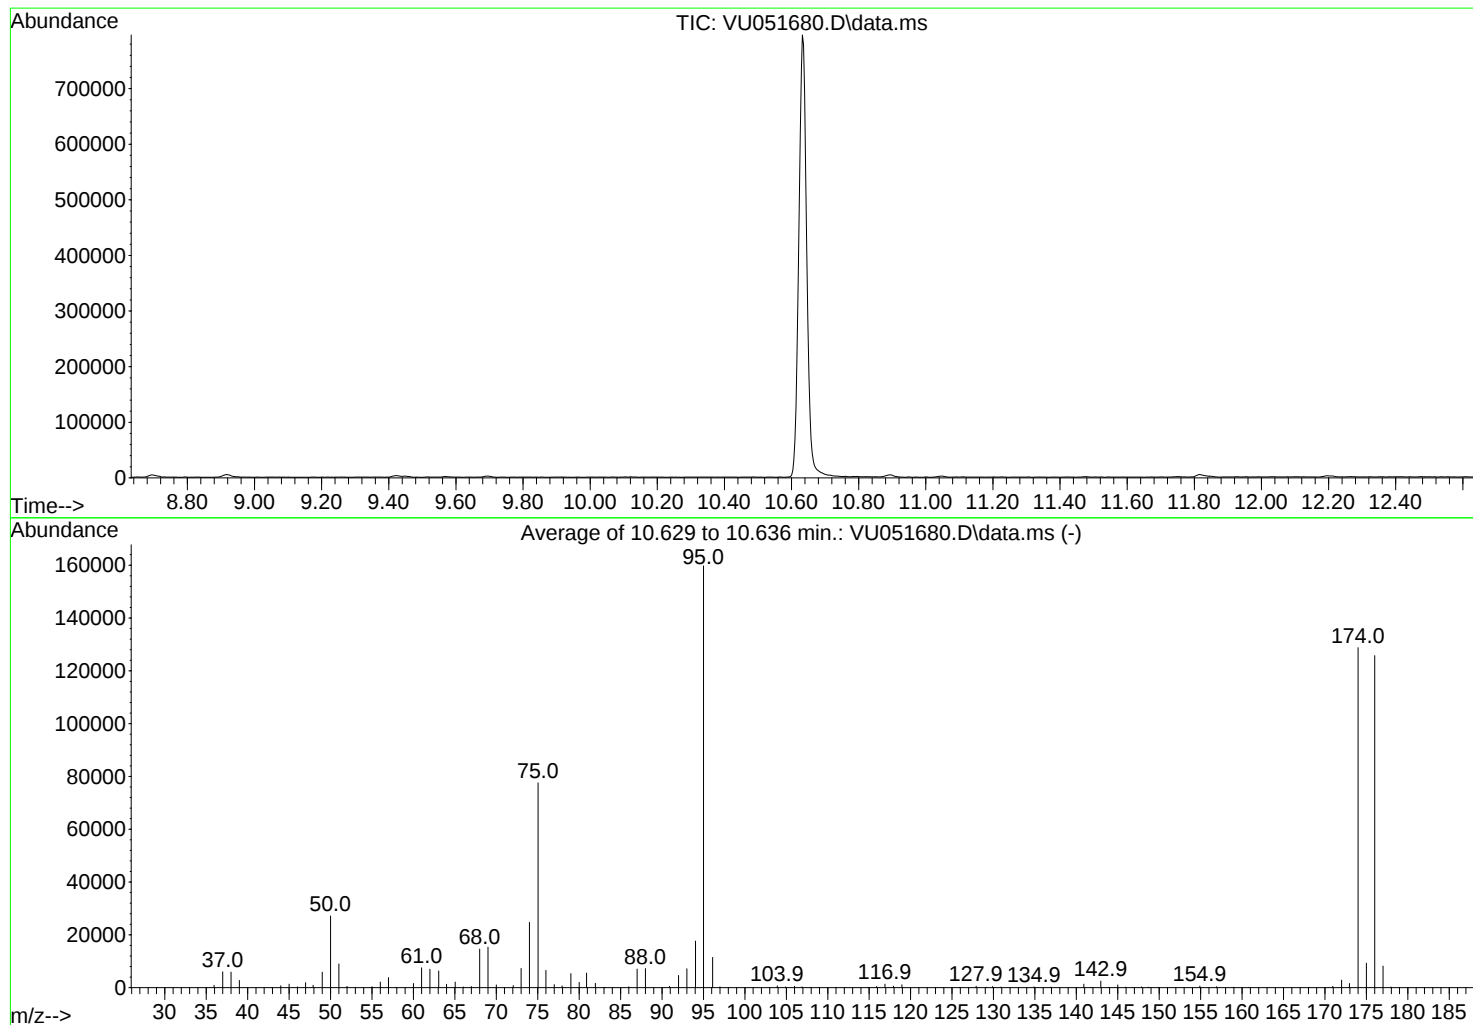

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	27136	PASS
75	95	30	80	48.5	77576	PASS
95	95	100	100	100.0	159787	PASS
96	95	5	9	7.2	11472	PASS
173	174	0.00	2	1.2	1563	PASS
174	95	50	120	80.6	128829	PASS
175	174	5	9	7.2	9274	PASS
176	174	95	101	97.6	125763	PASS
177	176	5	9	6.5	8215	PASS

Scan 2875 (10.584 min): VU051680.D\data.ms
BFB162

m/z	Abundance
40.00	824.0
44.00	641.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162

m/z	Abundance
35.90	956.0
37.00	5833.0
38.00	5961.0
39.00	2666.0
40.00	869.0
42.80	111.0
44.00	1357.0
45.00	1280.0
46.00	277.0
47.00	1789.0
47.90	944.0
49.00	5947.0
50.00	26432.0
51.00	8781.0
52.00	456.0
52.90	163.0
55.10	387.0
56.00	2249.0
57.00	3748.0
57.90	123.0
60.00	1741.0
61.00	7229.0
62.00	6619.0
63.00	6189.0
64.00	1283.0
65.10	2104.0
66.10	255.0
67.00	458.0
68.00	14142.0
69.00	14789.0
70.00	1030.0
72.10	757.0
73.00	6878.0
74.00	24264.0
75.00	75144.0
76.00	6378.0
77.00	1143.0
78.00	491.0
79.00	5448.0
80.00	1901.0
80.90	5399.0
81.90	1617.0
86.00	300.0
87.00	6589.0
88.00	6817.0
90.90	448.0
92.00	4288.0
93.00	6811.0
94.00	17072.0
95.00	154560.0
96.10	11049.0
97.00	364.0
103.90	725.0
104.90	263.0
106.00	570.0
106.90	300.0
107.90	138.0
111.00	113.0
113.00	138.0
114.80	252.0
115.90	445.0
116.90	1188.0
117.90	504.0
118.90	1083.0
123.90	100.0
125.90	103.0
127.90	498.0
129.10	208.0
129.90	406.0
130.90	193.0
134.90	281.0
137.00	232.0
140.90	1388.0
141.80	139.0
142.90	2495.0
143.90	126.0
145.00	1030.0
145.90	198.0
146.80	107.0
147.90	326.0
148.70	166.0
154.90	563.0
156.90	375.0
158.90	178.0
170.90	446.0
172.00	2608.0
173.00	1573.0
174.00	119800.0
175.00	8698.0
176.00	116832.0
177.00	7764.0
177.90	213.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162

m/z	Abundance
36.00	923.0
37.00	6234.0
38.00	6079.0
39.00	2845.0
39.90	900.0
42.90	123.0
44.00	1407.0
45.00	1355.0
46.00	336.0
47.00	1970.0
47.90	947.0
49.00	6097.0
50.00	28128.0
51.00	9364.0
52.00	500.0
53.00	172.0
55.00	380.0
56.00	2186.0
57.00	3949.0
57.90	108.0
60.00	1643.0
61.00	7860.0
62.00	7142.0
63.10	6534.0
64.00	1364.0
65.10	2243.0
66.10	249.0
67.00	450.0
68.00	15055.0
69.00	15839.0
70.00	1067.0
72.00	825.0
73.00	7504.0
74.00	25528.0
75.00	80232.0
76.00	6791.0
77.00	1225.0
77.90	693.0
79.00	5405.0
80.00	2080.0
80.90	5709.0
81.90	1739.0
83.00	109.0
86.00	319.0
87.00	7312.0
88.00	7543.0
90.90	510.0
92.00	4814.0
93.00	7491.0
94.10	18104.0
95.00	164928.0
96.10	12064.0
97.00	315.0
103.90	694.0
104.90	289.0
106.00	597.0
106.90	336.0
107.90	178.0
111.00	141.0
114.80	167.0
115.90	408.0
116.90	1398.0
118.00	545.0
118.90	1084.0
125.90	109.0
127.90	549.0
129.10	193.0
129.90	427.0
130.90	223.0
134.90	348.0
137.00	232.0
139.90	128.0
140.90	1422.0
141.80	152.0
143.00	2543.0
143.90	160.0
145.00	1062.0
145.90	240.0
146.80	118.0
147.90	332.0
148.70	184.0
149.90	123.0
152.80	114.0
154.90	640.0
156.90	353.0
158.90	193.0
160.80	108.0
171.00	527.0
172.00	2958.0
173.00	1626.0
174.00	132672.0
175.00	9593.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162

176.00	129872.0
177.00	8463.0
178.00	244.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162

m/z	Abundance
36.00	925.0
37.00	5970.0
38.00	5627.0
39.00	2730.0
39.90	888.0
44.00	1336.0
45.00	1309.0
46.00	334.0
47.00	1900.0
47.90	913.0
49.00	5644.0
50.00	26848.0
51.00	8774.0
52.00	472.0
53.10	192.0
54.90	427.0
56.00	1991.0
57.00	3777.0
57.90	105.0
60.00	1443.0
61.00	7499.0
62.00	7110.0
63.10	6249.0
64.00	1210.0
65.00	2118.0
66.00	213.0
67.00	430.0
68.00	14694.0
69.00	15468.0
70.00	1074.0
72.00	806.0
73.00	7465.0
74.00	24336.0
75.10	77352.0
76.00	6439.0
77.00	1137.0
77.90	785.0
79.00	5109.0
80.00	2008.0
80.90	5480.0
82.00	1649.0
86.00	306.0
87.00	7255.0
88.00	7326.0
90.90	508.0
92.00	4779.0
93.00	7209.0
94.10	17760.0
95.00	159872.0
96.10	11302.0
97.00	287.0
103.90	600.0
104.90	290.0
106.00	555.0
106.90	269.0
108.00	162.0
111.00	117.0
115.00	129.0
115.90	401.0
116.90	1362.0
117.90	554.0
119.00	1081.0
127.90	521.0
129.10	182.0
129.90	414.0
130.90	235.0
134.90	338.0
136.90	207.0
139.90	118.0
140.90	1278.0
141.80	149.0
143.00	2376.0
143.80	188.0
145.00	1023.0
146.00	278.0
147.80	300.0
148.70	181.0
149.90	180.0
152.90	150.0
154.90	599.0
156.90	323.0
159.00	175.0
160.80	113.0
171.00	518.0
172.00	3013.0
172.90	1490.0
174.00	134016.0
175.00	9530.0
176.00	130584.0
177.00	8419.0
178.00	227.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162