

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112222\
 Data File : VU052058.D
 Acq On : 22 Nov 2022 22:57
 Operator : JC/MD
 Sample : N5693-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBN94

Quant Time: Nov 23 00:50:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 19 21:39:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	214411	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	225259	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	82665	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	100683	4.828	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.600%
7) Chloroethane-d5	1.912	69	83963	5.183	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.600%
11) 1,1-Dichloroethene-d2	2.565	65	36030	4.820	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	96.400%
20) 2-Butanone-d5	4.629	46	195657	51.756	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.520%
24) Chloroform-d	5.060	84	159785	5.214	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.200%
26) 1,2-Dichloroethane-d4	5.700	65	83016	5.363	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.200%
32) Benzene-d6	5.726	84	328622	4.914	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
36) 1,2-Dichloropropane-d6	6.687	67	106931	5.167	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.400%
41) Toluene-d8	7.896	98	251929	4.164	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.200%
43) trans-1,3-Dichloroprop...	8.179	79	28170	3.735	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.800%
46) 2-Hexanone-d5	8.632	63	138524	43.341	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.680%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	86950	4.846	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.000%
66) 1,2-Dichlorobenzene-d4	12.192	152	87393	5.522	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.400%
Target Compounds					Qvalue	
13) Acetone	2.642	43	7027	2.737	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112222\
Data File : VU052058.D
Acq On : 22 Nov 2022 22:57
Operator : JC/MD
Sample : N5693-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBN94

Quant Time: Nov 23 00:50:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 19 21:39:41 2022
Response via : Initial Calibration

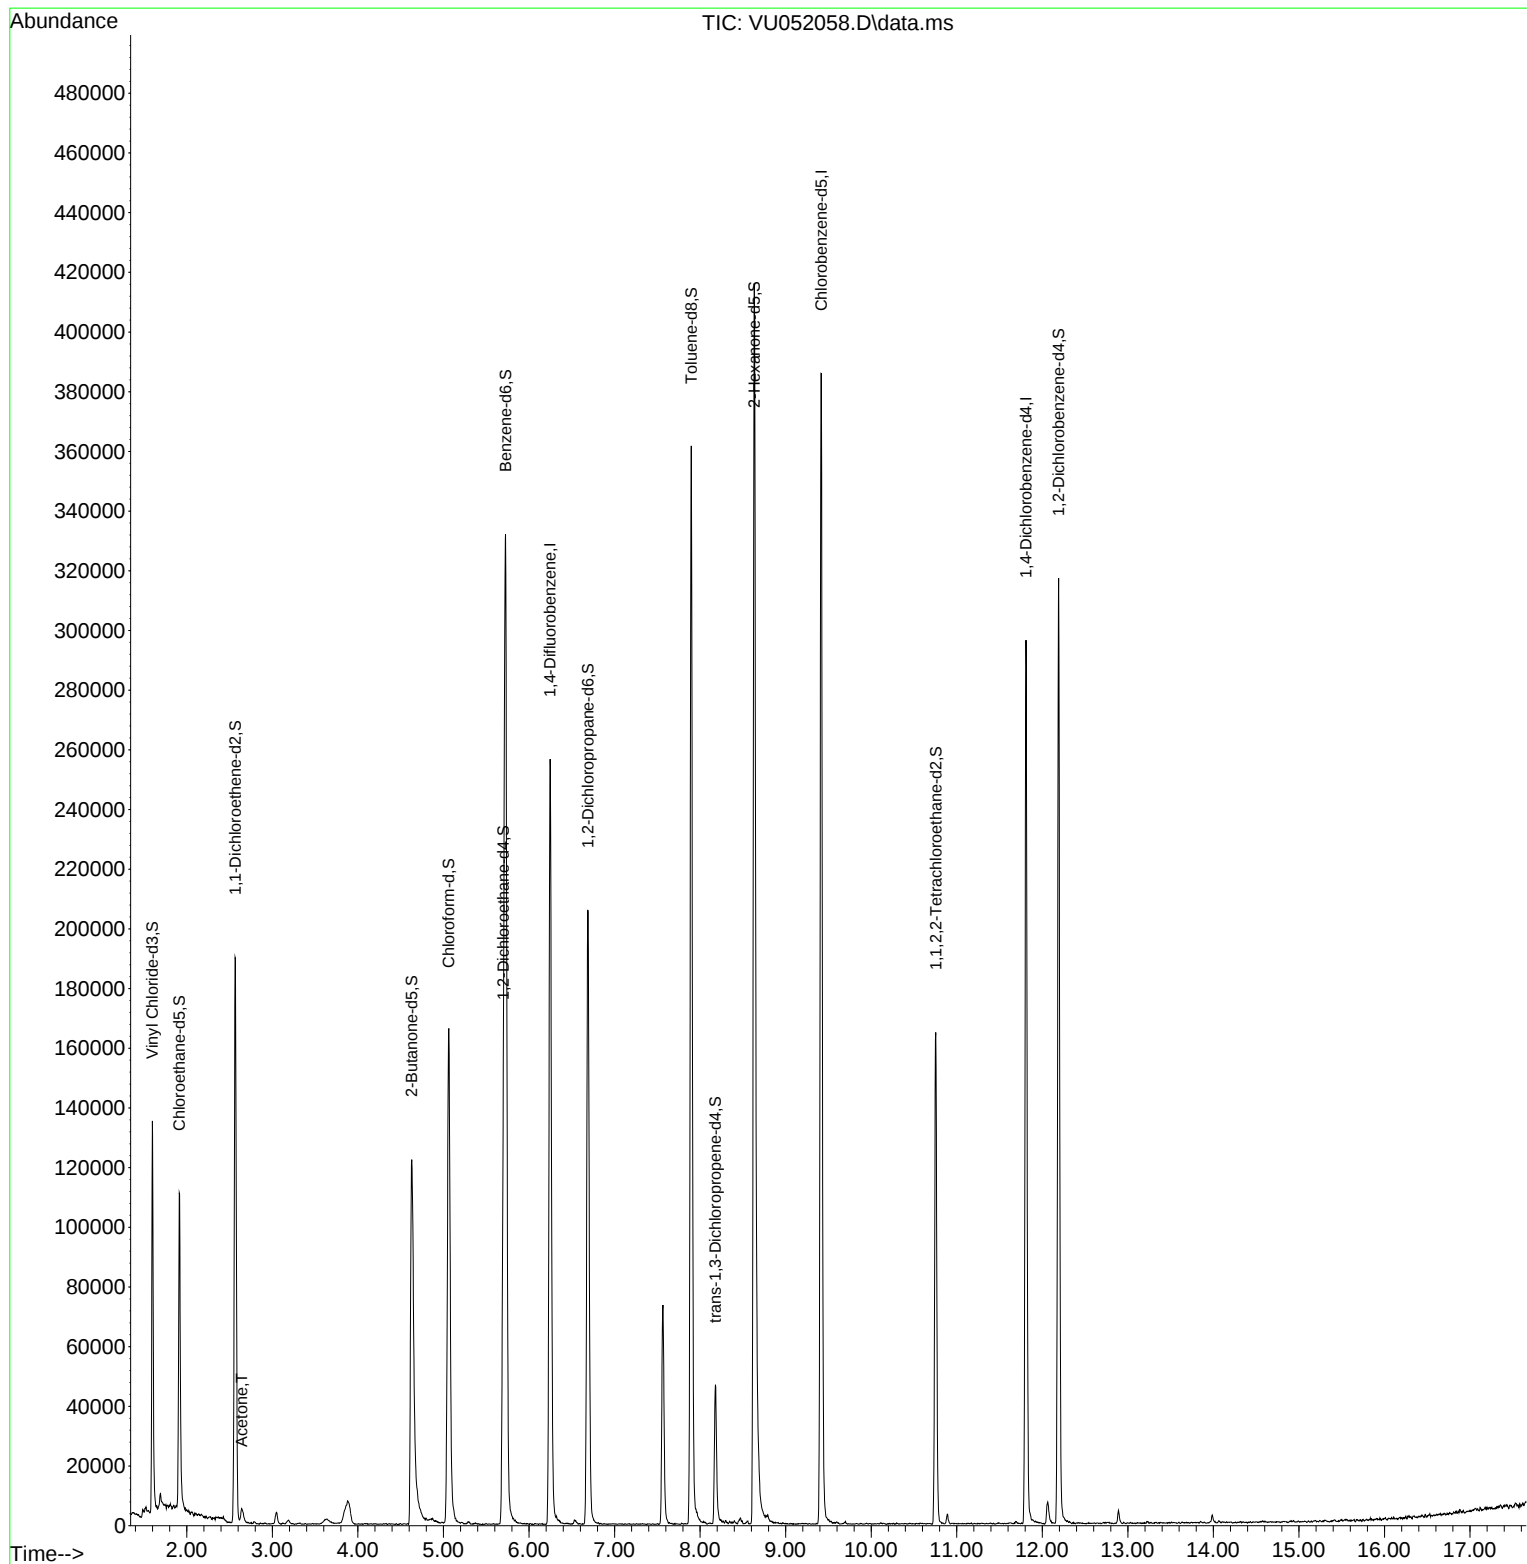

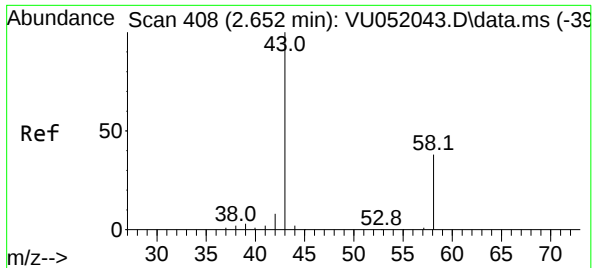

#13
 Acetone
 Concen: 2.737 ug/L
 RT: 2.642 min Scan# 40
 Delta R.T. 0.023 min
 Lab File: VU052058.D
 Acq: 22 Nov 2022 22:57

Instrument :
 MSVOA_U
 ClientSampleId :
 GBN94

Tgt Ion: 43 Resp: 7027
 Ion Ratio Lower Upper
 43 100
 58 32.3 0.0 76.0

