

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112222\
 Data File : VU052076.D
 Acq On : 23 Nov 2022 08:01
 Operator : JC/MD
 Sample : N5693-12DL 400X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBN93DL

Quant Time: Nov 23 08:26:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 19 21:39:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	209453	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	215938	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	81055	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	95526	4.689	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.800%	
7) Chloroethane-d5	1.916	69	80244	5.071	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.400%	
11) 1,1-Dichloroethene-d2	2.565	65	36512	5.000	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	100.000%	
20) 2-Butanone-d5	4.639	46	218463	59.156	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	118.320%	
24) Chloroform-d	5.060	84	163296	5.455	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	109.000%	
26) 1,2-Dichloroethane-d4	5.700	65	85558	5.659	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	113.200%	
32) Benzene-d6	5.726	84	337576	5.266	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	105.400%	
36) 1,2-Dichloropropane-d6	6.690	67	110335	5.561	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	111.200%	
41) Toluene-d8	7.896	98	264900	4.567	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.400%	
43) trans-1,3-Dichloroprop...	8.179	79	34380	4.755	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.200%	
46) 2-Hexanone-d5	8.633	63	160099	52.253	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	104.500%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	94400	5.488	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	109.800%	
66) 1,2-Dichlorobenzene-d4	12.192	152	90778	5.850	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	117.000%	
Target Compounds						
						Qvalue
16) Methylene chloride	3.048	84	8569	0.417	ug/L	97
22) cis-1,2-Dichloroethene	4.665	96	20703	1.211	ug/L	91
34) Trichloroethene	6.539	95	92409	5.272	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112222\
Data File : VU052076.D
Acq On : 23 Nov 2022 08:01
Operator : JC/MD
Sample : N5693-12DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBN93DL

Quant Time: Nov 23 08:26:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 19 21:39:41 2022
Response via : Initial Calibration




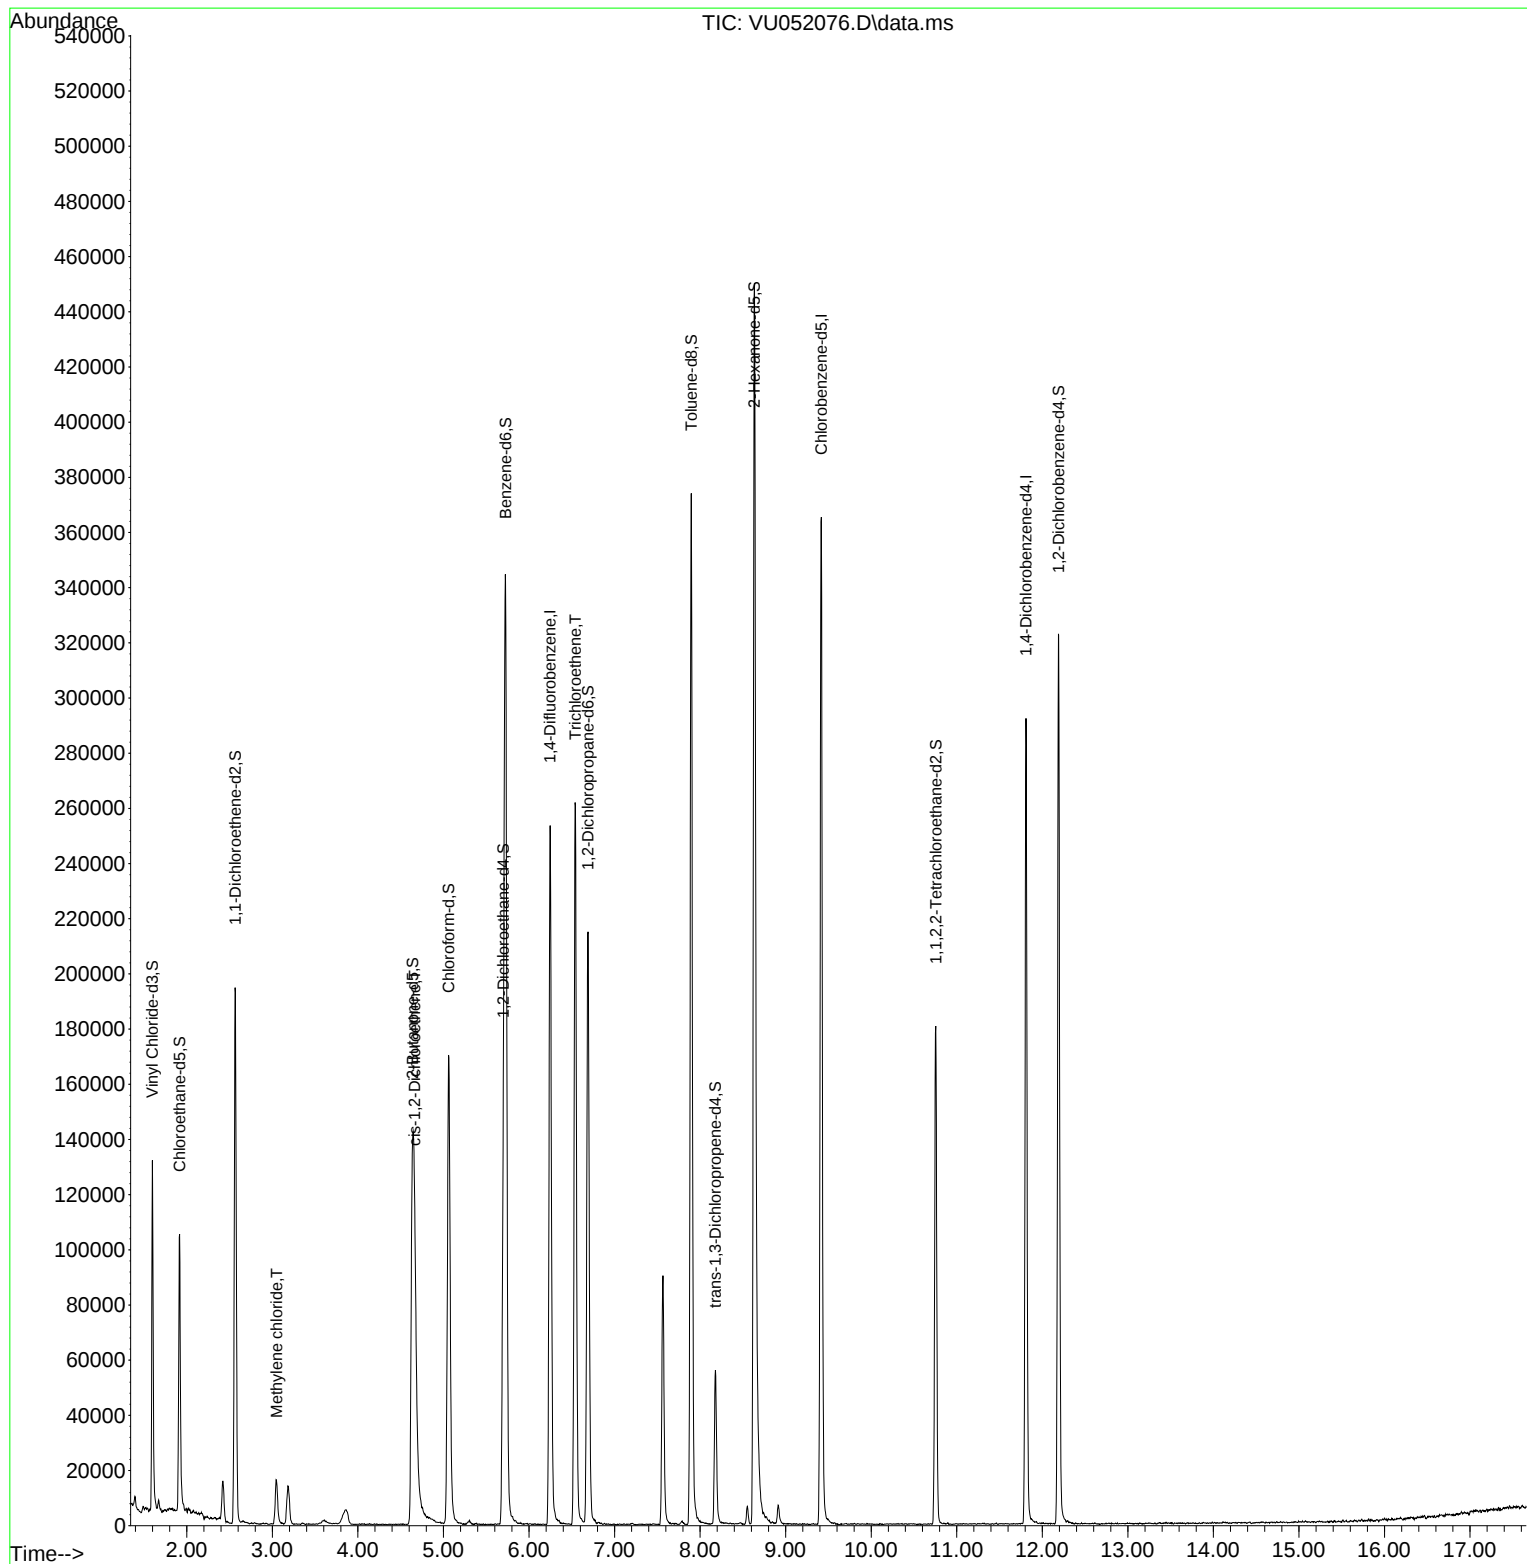


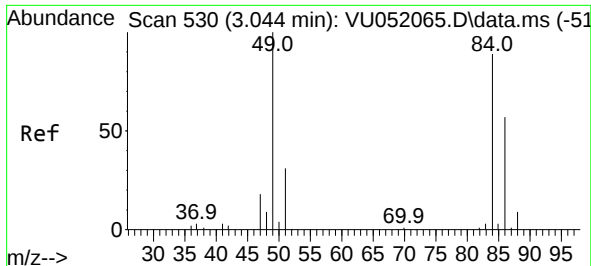

#16
Methylene chloride
Concen: 0.417 ug/L
RT: 3.048 min Scan# 51
Delta R.T. 0.003 min
Lab File: VU052076.D
Acq: 23 Nov 2022 08:01




Instrument :
MSVOA_U
ClientSampleId :
GBN93DL


Tgt Ion: 84 Resp: 8569
Ion Ratio Lower Upper
84 100
86 68.1 43.8 81.4
49 109.8 75.9 141.1

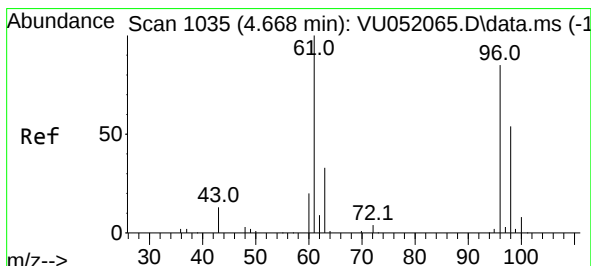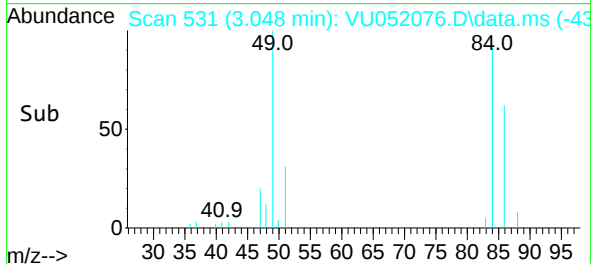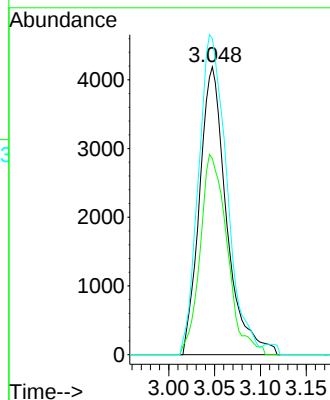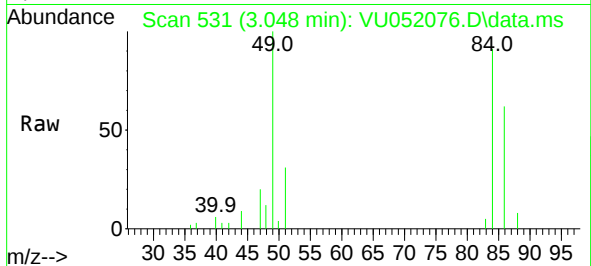

#22
cis-1,2-Dichloroethene
Concen: 1.211 ug/L
RT: 4.665 min Scan# 1034
Delta R.T. 0.000 min
Lab File: VU052076.D
Acq: 23 Nov 2022 08:01

Tgt Ion: 96 Resp: 20703
Ion Ratio Lower Upper
96 100
61 133.4 85.1 158.1
98 65.1 42.8 79.6

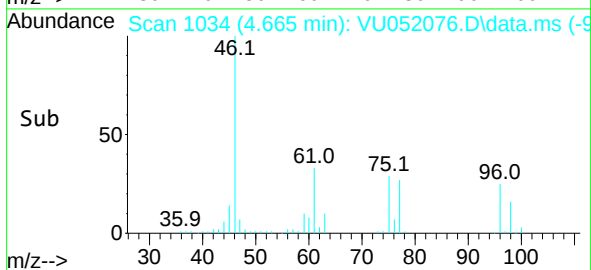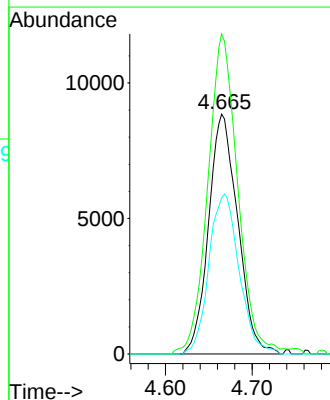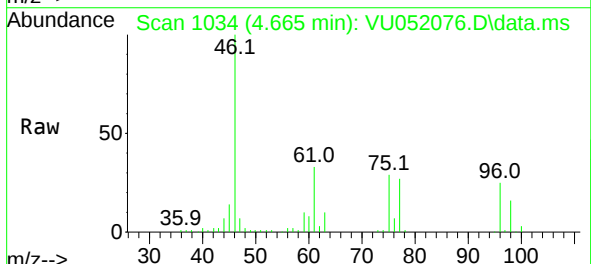

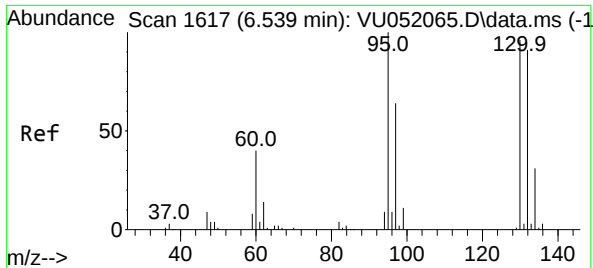

#34
 Trichloroethene
 Concen: 5.272 ug/L
 RT: 6.539 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU052076.D
 Acq: 23 Nov 2022 08:01

Instrument :
 MSVOA_U
 ClientSampleId :
 GBN93DL

Tgt Ion: 95	Resp:	92409
Ion	Ratio	Lower Upper
95	100	
97	66.0	43.7 81.1
132	97.7	64.3 119.3
130	99.9	67.3 124.9

