

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112222\
 Data File : VU052066.D
 Acq On : 23 Nov 2022 03:02
 Operator : JC/MD
 Sample : VU1122WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK144

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052066.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	104	rVB	119126	144591	16.44%	2.107%
2	1.916	170	179	202	rVB	97871	140499	15.98%	2.047%
3	2.568	369	382	397	rBV	185582	299942	34.11%	4.371%
4	3.047	518	531	546	rBV	18278	34006	3.87%	0.496%
5	3.182	562	573	584	rBV2	4725	9315	1.06%	0.136%
6	3.838	753	777	800	rVB	6341	22584	2.57%	0.329%
7	4.636	1011	1025	1071	rBV	123847	384583	43.73%	5.604%
8	5.063	1142	1158	1182	rBV	165630	374214	42.55%	5.453%
9	5.723	1339	1363	1384	rBV2	334010	870854	99.02%	12.690%
10	6.247	1508	1526	1549	rBV	258203	493273	56.09%	7.188%
11	6.690	1649	1664	1682	rBV	209469	413961	47.07%	6.032%
12	7.565	1924	1936	1957	rBV	87308	160233	18.22%	2.335%
13	7.896	2026	2039	2068	rBV	359080	640479	72.83%	9.333%
14	8.179	2113	2127	2144	rBV	55690	96227	10.94%	1.402%
15	8.636	2257	2269	2301	rBV2	432075	879444	100.00%	12.816%
16	9.417	2498	2512	2539	rBV	376708	640175	72.79%	9.329%
17	10.754	2914	2928	2945	rBV	170709	278291	31.64%	4.055%
18	11.809	3243	3256	3274	rBV	289510	466430	53.04%	6.797%
19	12.192	3362	3375	3399	rBV	306016	513153	58.35%	7.478%




Sum of corrected areas: 6862254

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112222\
Data File : VU052066.D
Acq On : 23 Nov 2022 03:02
Operator : JC/MD
Sample : VU1122WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

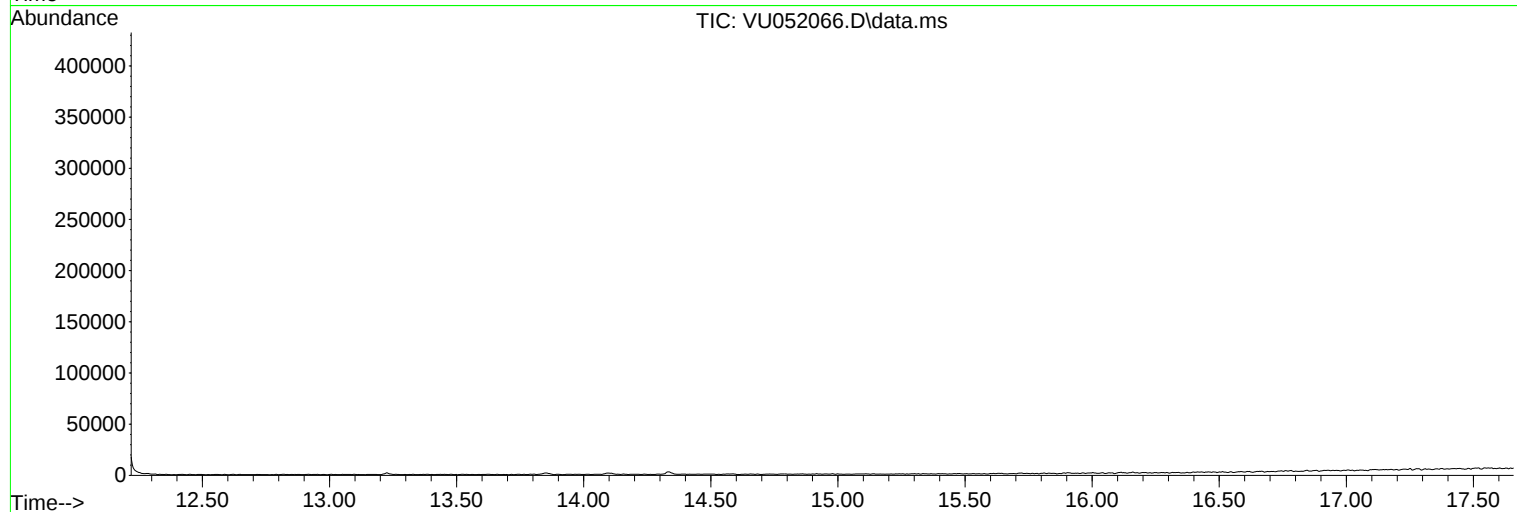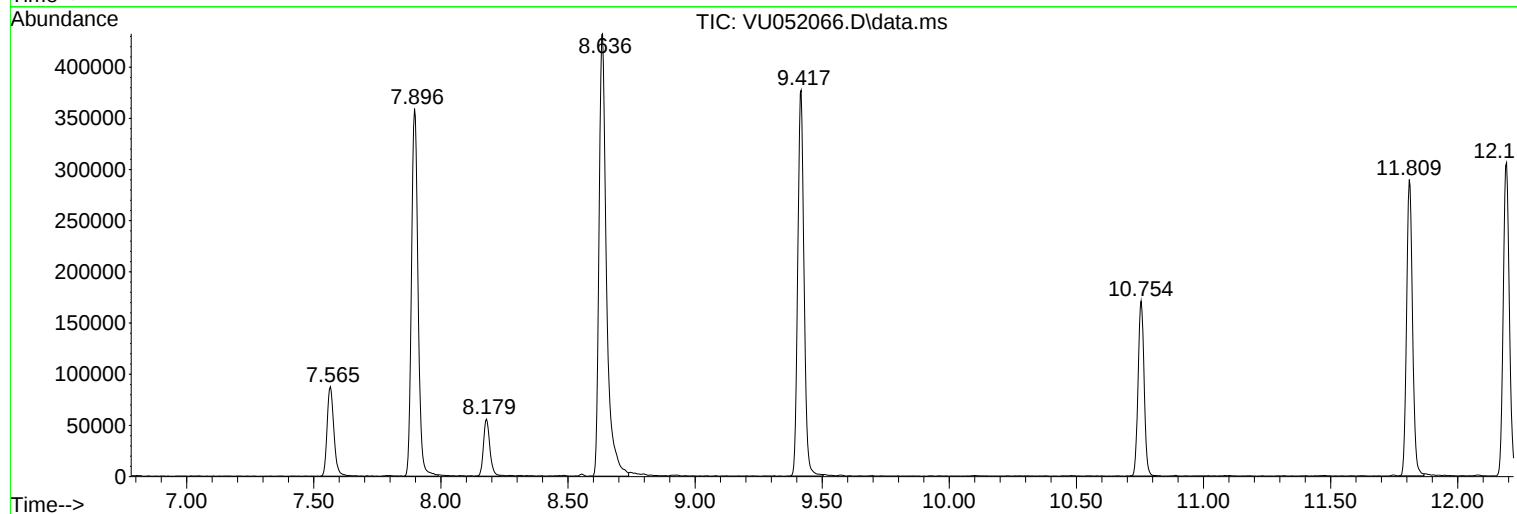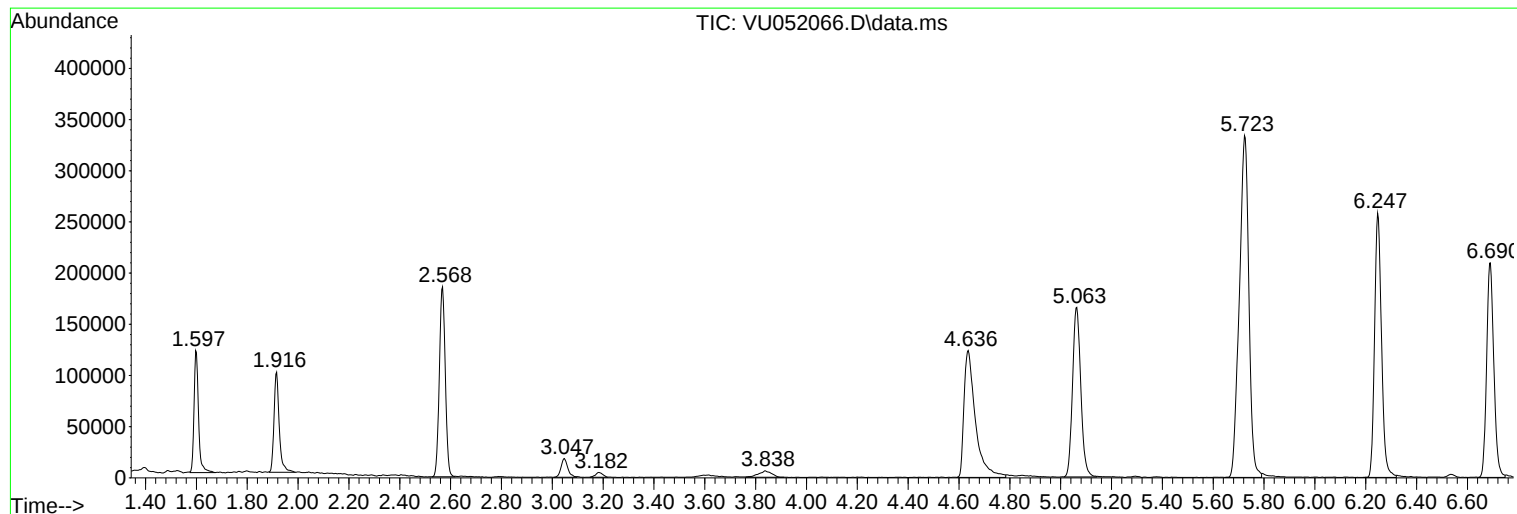

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112222\
Data File : VU052066.D
Acq On : 23 Nov 2022 03:02
Operator : JC/MD
Sample : VU1122WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112222\
Data File : VU052066.D
Acq On : 23 Nov 2022 03:02
Operator : JC/MD
Sample : VU1122WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc