


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112222\
 Data File : VU052042.D
 Acq On : 22 Nov 2022 14:59
 Operator : JC/MD
 Sample : BFB171
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB171

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Nov 24 05:20:45 2022

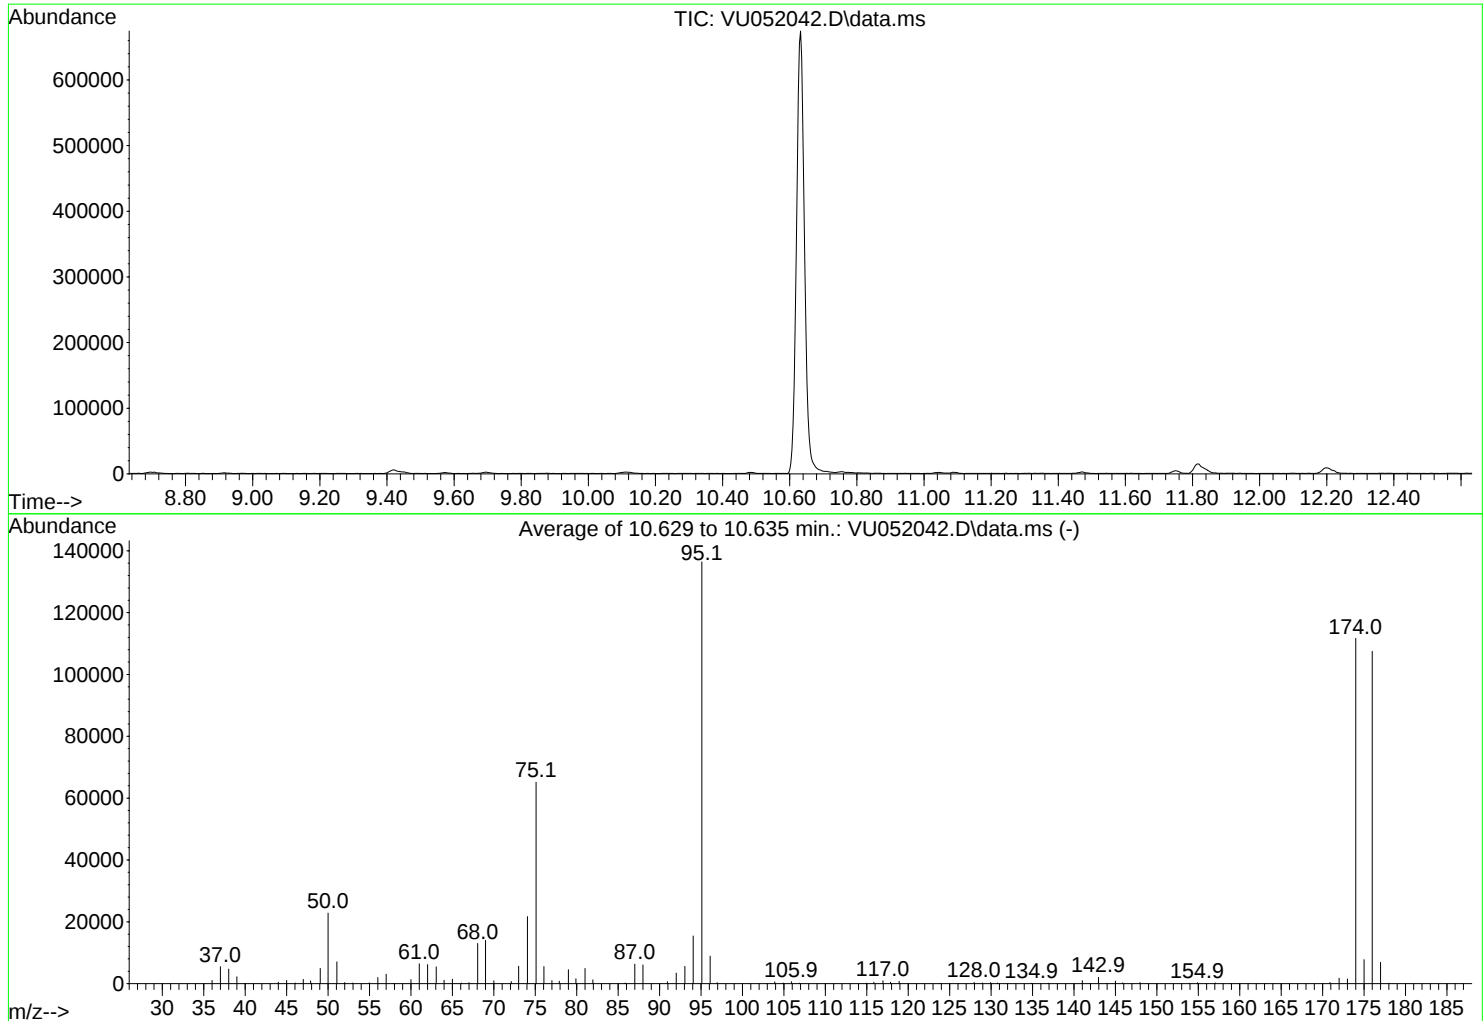

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	22824	PASS
75	95	30	80	47.8	65181	PASS
95	95	100	100	100.0	136421	PASS
96	95	5	9	6.5	8923	PASS
173	174	0.00	2	1.4	1512	PASS
174	95	50	120	81.9	111672	PASS
175	174	5	9	7.0	7786	PASS
176	174	95	101	96.2	107464	PASS
177	176	5	9	6.4	6911	PASS

m/z	Abundance
35.90	1570.0
38.00	486.0
39.90	177.0
43.90	466.0

Instrument :
MSVOA_U
ClientSampleId :
BFB171

m/z	Abundance
36.00	2425.0
37.00	4822.0
38.00	4837.0
39.00	2257.0
39.90	379.0
44.00	1217.0
45.00	836.0
46.00	157.0
47.00	1423.0
48.00	733.0
49.00	4480.0
50.00	21240.0
51.00	6913.0
52.10	407.0
53.00	175.0
53.90	137.0
54.90	344.0
56.00	1528.0
57.00	3288.0
57.90	131.0
60.00	1136.0
61.00	5825.0
62.00	6528.0
63.00	5363.0
64.00	994.0
65.00	1335.0
66.00	256.0
67.00	366.0
68.00	12346.0
69.00	11664.0
70.00	851.0
72.00	598.0
73.00	5366.0
74.00	20008.0
75.00	60840.0
76.00	5539.0
77.00	945.0
77.80	534.0
78.90	4433.0
80.00	1329.0
81.00	4777.0
81.90	1085.0
85.90	262.0
87.00	5388.0
88.00	4805.0
90.90	407.0
92.10	3212.0
93.00	5751.0
94.00	14542.0
95.00	125496.0
96.00	8343.0
97.10	190.0
103.90	596.0
104.90	120.0
105.90	592.0
111.00	147.0
111.90	133.0
114.90	151.0
115.80	522.0
116.90	957.0
117.90	389.0
118.90	748.0
127.80	520.0
128.90	125.0
129.90	433.0
131.00	186.0
134.90	301.0
136.90	178.0
141.00	1050.0
142.00	188.0
143.00	1898.0
143.90	151.0
144.90	830.0
145.90	247.0
148.00	232.0
149.90	117.0
153.90	117.0
154.90	291.0
157.00	198.0
160.80	102.0
170.90	293.0
172.00	2164.0
173.00	1249.0
174.00	101776.0
175.00	7639.0
176.00	97952.0
177.00	6387.0
178.00	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB171

m/z	Abundance
36.00	2227.0
37.00	4695.0
38.00	4897.0
39.00	2247.0
39.90	338.0
44.00	1116.0
45.00	867.0
45.90	153.0
47.00	1470.0
48.00	667.0
49.00	4425.0
50.00	20536.0
51.00	6867.0
52.10	362.0
53.00	154.0
53.90	133.0
54.90	353.0
56.00	1594.0
57.00	3095.0
60.00	1214.0
61.00	5607.0
62.00	6110.0
63.00	5384.0
64.00	874.0
65.00	1208.0
66.00	266.0
67.00	377.0
68.00	11824.0
69.00	11175.0
70.10	752.0
72.00	641.0
73.00	5280.0
74.00	19496.0
75.00	58648.0
76.10	5189.0
77.00	877.0
77.80	416.0
79.00	4206.0
80.00	1284.0
81.00	4769.0
81.90	1039.0
85.90	246.0
87.00	5445.0
88.00	4703.0
90.90	412.0
92.10	3043.0
93.00	5398.0
94.10	13839.0
95.10	122256.0
96.00	8158.0
97.10	203.0
103.90	666.0
104.90	120.0
105.90	652.0
106.80	110.0
111.00	156.0
112.00	100.0
114.90	167.0
115.90	517.0
116.90	866.0
117.90	354.0
118.90	888.0
127.80	481.0
128.90	147.0
129.90	477.0
131.00	244.0
134.90	264.0
136.90	159.0
141.00	1107.0
141.90	140.0
143.00	1821.0
143.90	190.0
144.90	841.0
145.80	228.0
148.00	227.0
149.90	132.0
154.90	361.0
157.00	207.0
159.00	117.0
160.90	122.0
170.90	238.0
172.00	2198.0
173.00	1204.0
174.00	102704.0
175.00	7717.0
176.00	97976.0
176.90	6189.0
178.00	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB171

m/z	Abundance
36.00	998.0
37.00	5208.0
38.00	4528.0
39.00	2162.0
39.90	283.0
44.00	941.0
45.00	899.0
46.00	223.0
47.00	1331.0
47.90	827.0
49.00	4419.0
50.00	21768.0
51.10	6786.0
52.00	315.0
52.90	215.0
54.90	228.0
56.00	1908.0
57.00	2754.0
57.80	136.0
60.00	1288.0
61.00	6059.0
62.00	6096.0
63.00	4920.0
64.00	1060.0
65.00	1456.0
66.00	124.0
67.00	315.0
68.10	12470.0
69.00	13097.0
70.00	867.0
72.10	636.0
73.00	5429.0
74.00	20912.0
75.10	62208.0
76.00	5291.0
77.00	949.0
77.90	671.0
79.00	4353.0
79.90	1637.0
81.00	4726.0
82.00	1185.0
85.90	151.0
87.00	6107.0
88.00	5775.0
90.90	553.0
92.00	3289.0
93.10	5537.0
94.10	15099.0
95.10	130992.0
96.10	8655.0
96.90	267.0
103.90	540.0
104.90	221.0
105.90	599.0
106.90	153.0
115.00	117.0
115.90	433.0
117.00	990.0
117.80	493.0
118.90	644.0
123.90	100.0
127.90	408.0
128.90	278.0
130.00	378.0
130.80	234.0
135.00	203.0
136.90	160.0
141.00	1028.0
142.00	130.0
142.90	1861.0
143.90	115.0
145.00	764.0
145.80	243.0
147.90	369.0
153.90	139.0
154.90	386.0
157.00	182.0
158.90	104.0
161.00	107.0
170.90	346.0
172.00	1699.0
173.00	1415.0
174.00	110304.0
175.00	7526.0
176.00	106576.0
177.00	6907.0
178.00	144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB171