

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010220\
 Data File : VU036390.D
 Acq On : 02 Jan 2020 12:59
 Operator : JC/MD
 Sample : K6459-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Jan 03 00:57:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 03 00:45:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	280296	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	265738	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	112534	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	82487	4.05	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.00%
7) Chloroethane-d5	1.93	69	81223	4.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.00%
11) 1,1-Dichloroethene-d2	2.59	63	130167	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	4.70	46	251033	48.33	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.66%
24) Chloroform-d	5.11	84	192528	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
26) 1,2-Dichloroethane-d4	5.75	65	106534	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.80%
32) Benzene-d6	5.77	84	377496	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
36) 1,2-Dichloropropane-d6	6.73	67	123891	5.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.80%
41) Toluene-d8	7.93	98	339632	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.00%
43) trans-1,3-Dichloropropene-	8.21	79	54614	4.81	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.20%
46) 2-Hexanone-d5	8.68	63	266487	54.61	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.22%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	107078	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.40%
64) 1,2-Dichlorobenzene-d4	12.22	152	118154	4.92	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.40%


Target Compounds					Ovalue
13) Acetone	2.68	43	9704	2.900	ug/L 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU010220\
Data File : VU036390.D
Acq On : 02 Jan 2020 12:59
Operator : JC/MD
Sample : K6459-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Jan 03 00:57:55 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 03 00:45:06 2020
Response via : Initial Calibration

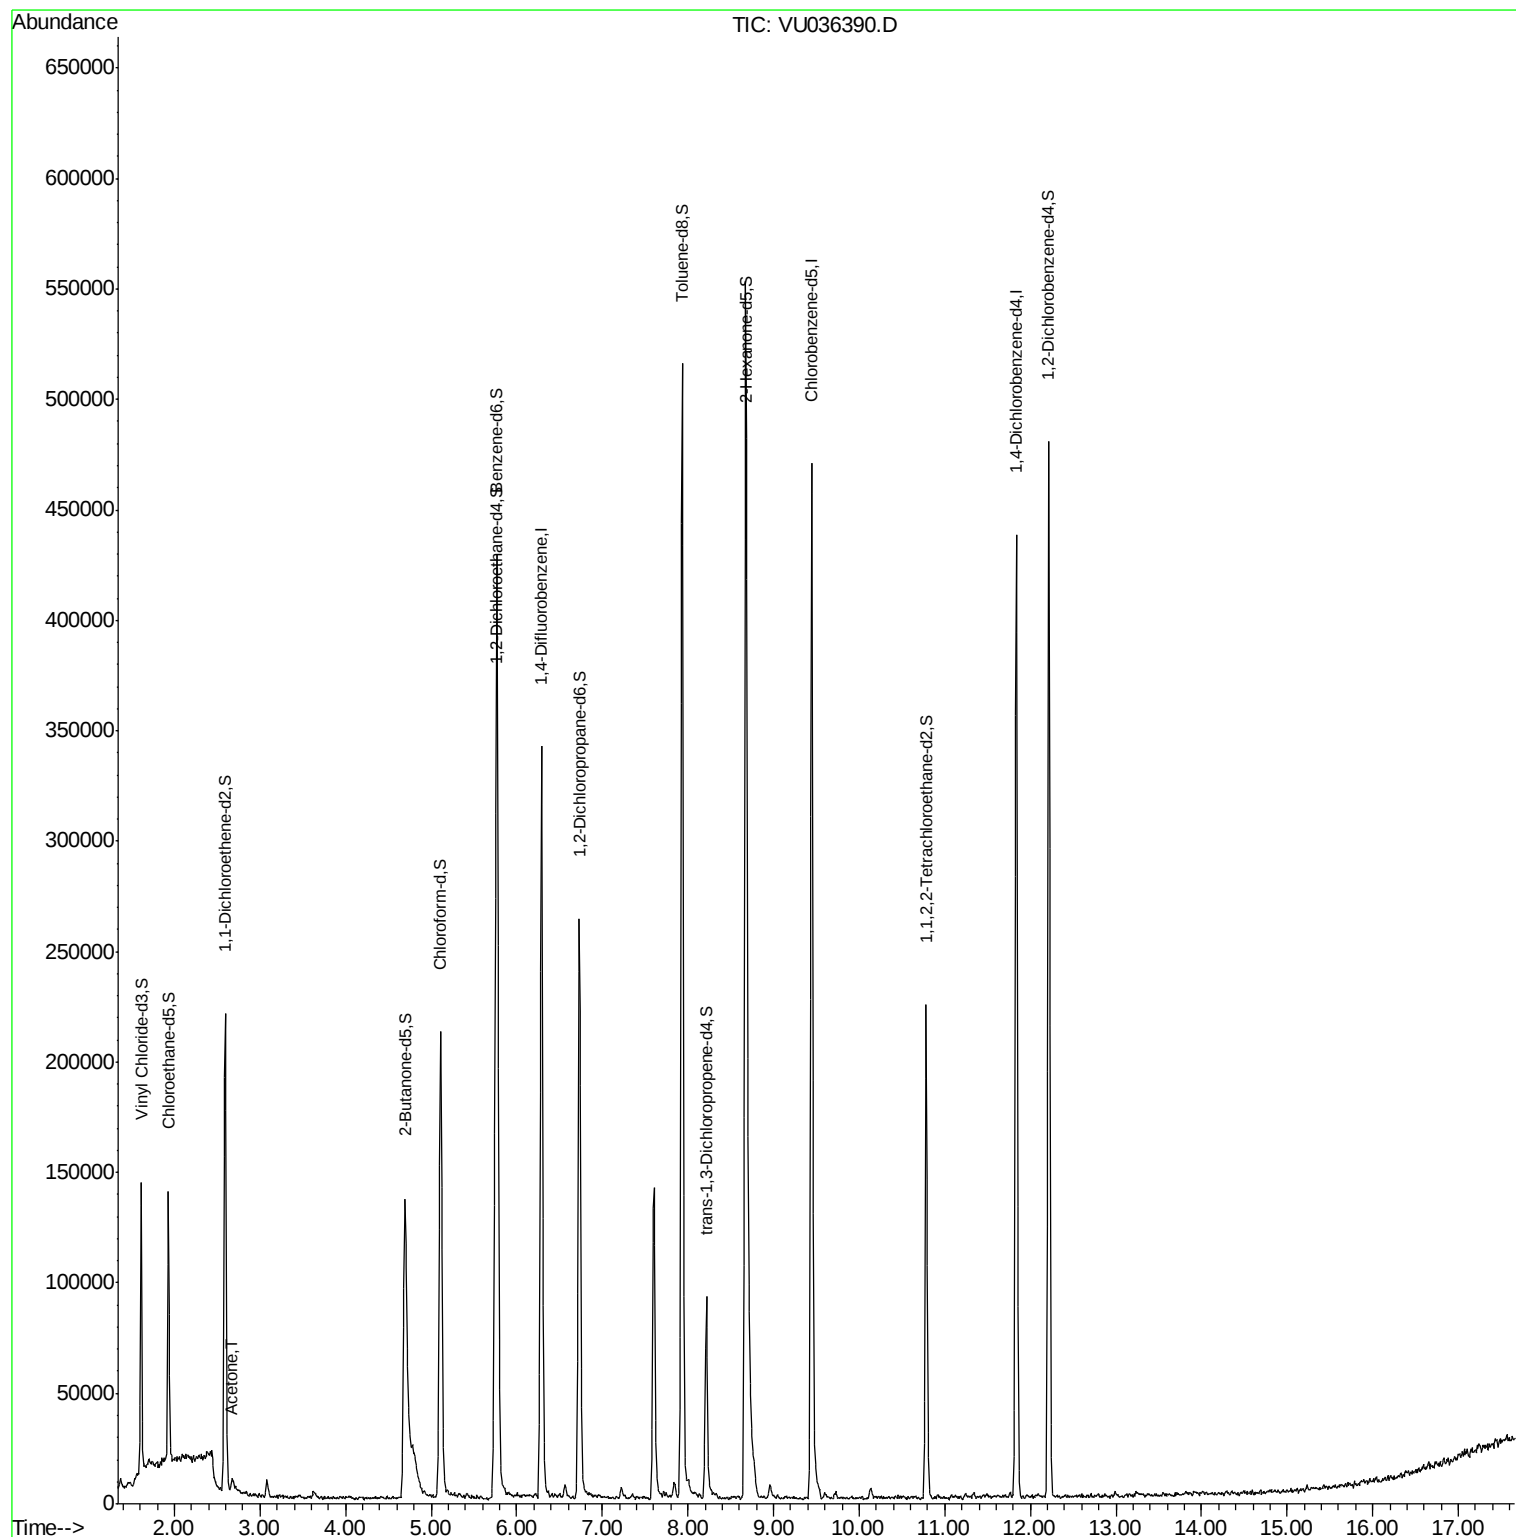

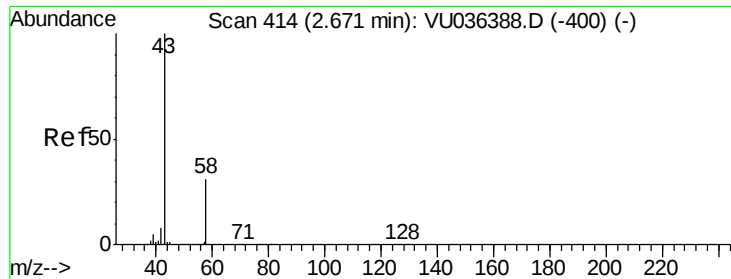

#13

Acetone

Concen: 2.900 ug/L

RT: 2.68 min Scan# 416

Delta R.T. 0.01 min

Lab File: VU036390.D

Acq: 02 Jan 2020 12:59

Instrument :

MSVOA_U

ClientSampleId :

VHBLK01

Tot Ion: 43 Resp: 9704

Ion Ratio Lower Upper

43 100

58 28.3 0.0 57.0

