
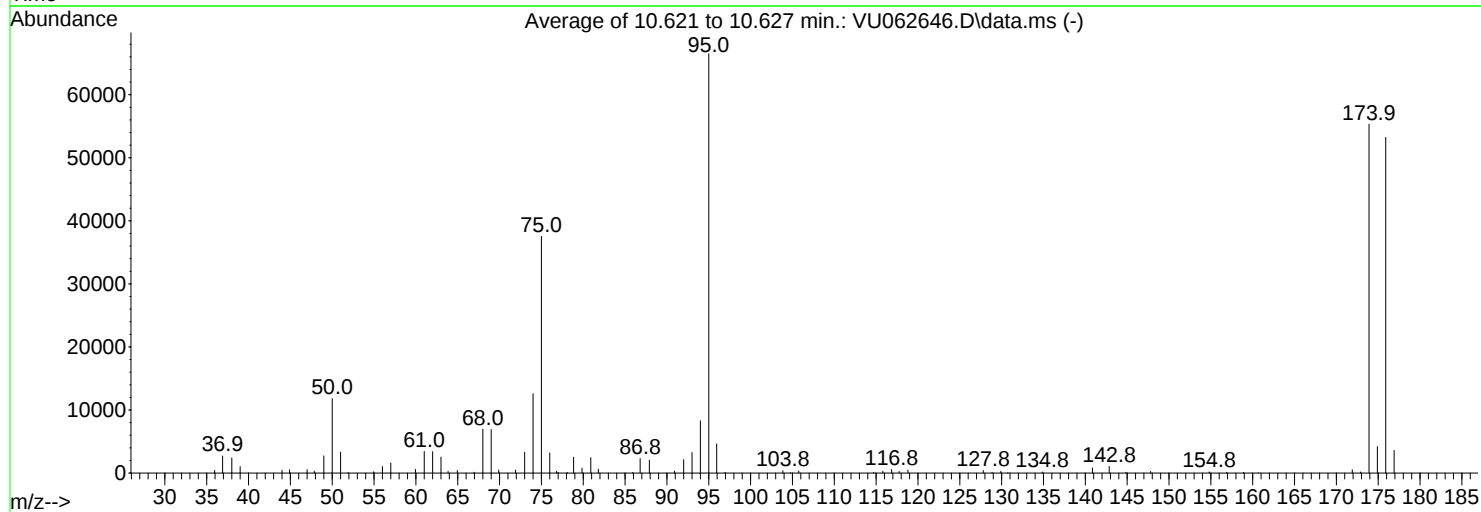


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010225\
Data File : VU062646.D
Acq On : 02 Jan 2025 08:50
Operator : MD/SY
Sample : BFB057
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB057

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jan 03 00:48:41 2025

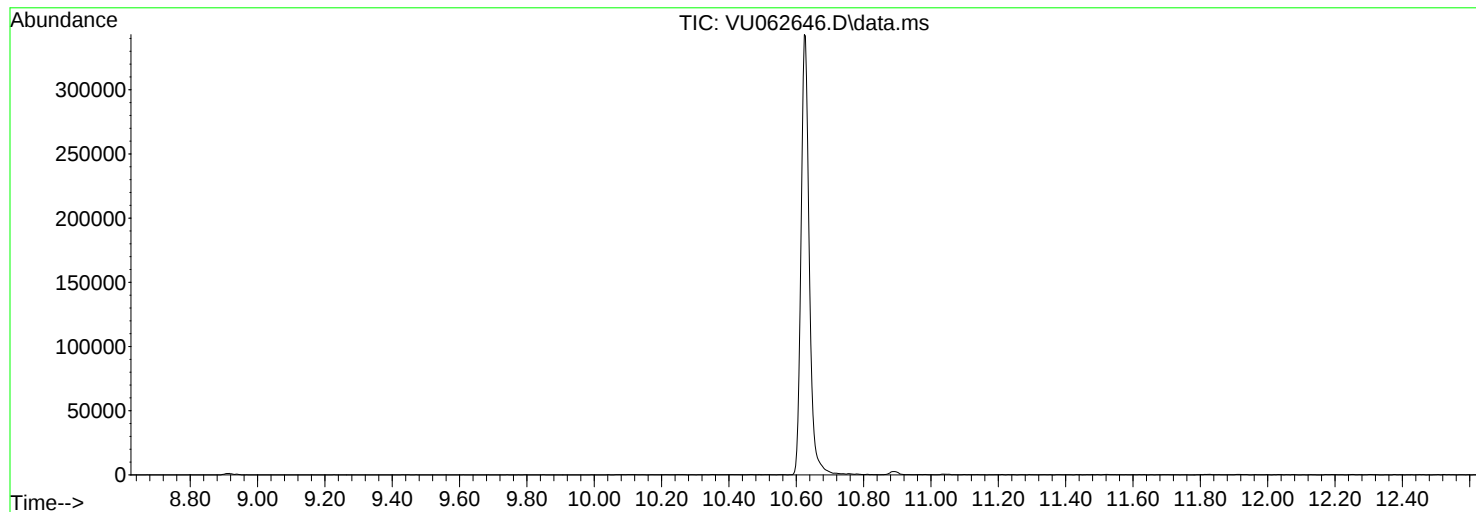

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	11791	PASS
75	95	30	80	56.5	37541	PASS
95	95	100	100	100.0	66496	PASS
96	95	5	9	7.0	4630	PASS
173	174	0.00	2	0.3	185	PASS
174	95	50	120	83.2	55331	PASS
175	174	5	9	7.6	4207	PASS
176	174	95	101	96.2	53229	PASS
177	176	5	9	6.8	3596	PASS

m/z	Abundance
35.80	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
36.00	586.0
36.90	2561.0
38.00	2257.0
39.00	1068.0
44.00	405.0
44.90	518.0
47.00	480.0
47.90	309.0
49.00	2559.0
50.00	11477.0
51.00	3153.0
55.00	193.0
56.00	1002.0
57.00	1530.0
60.00	617.0
61.00	3298.0
62.00	3201.0
63.00	2422.0
63.80	243.0
65.00	419.0
67.00	199.0
68.00	6627.0
69.00	6562.0
69.90	460.0
71.90	470.0
73.00	3204.0
74.00	11922.0
75.00	35664.0
76.00	3046.0
76.80	435.0
78.80	2305.0
79.80	701.0
80.90	2290.0
81.80	567.0
85.90	104.0
86.80	2148.0
87.90	1934.0
90.90	305.0
92.00	1945.0
93.00	3006.0
94.00	7836.0
95.00	62248.0
96.00	4429.0
96.90	131.0
103.90	321.0
105.80	317.0
114.60	107.0
115.80	280.0
116.80	481.0
117.80	261.0
118.80	447.0
127.80	516.0
128.80	121.0
129.90	267.0
134.90	200.0
140.90	742.0
142.80	930.0
144.80	136.0
147.80	253.0
154.80	143.0
156.80	109.0
158.90	120.0
171.90	422.0
173.90	50600.0
174.90	4118.0
175.90	48880.0
176.90	3335.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
36.00	607.0
36.90	2777.0
38.00	2477.0
39.00	1086.0
44.00	468.0
44.90	545.0
47.00	609.0
47.90	333.0
49.00	2860.0
50.00	12287.0
51.00	3411.0
51.90	108.0
54.90	225.0
56.00	1055.0
57.00	1683.0
60.00	581.0
61.00	3557.0
62.00	3484.0
63.00	2598.0
63.90	285.0
64.90	445.0
66.90	234.0
68.00	7200.0
69.00	7080.0
69.90	501.0
71.90	508.0
73.00	3465.0
74.00	13132.0
75.00	38728.0
76.00	3354.0
76.80	389.0
78.90	2625.0
79.80	855.0
80.90	2570.0
81.80	642.0
85.90	103.0
86.80	2455.0
87.90	2129.0
90.90	324.0
92.00	2228.0
93.00	3358.0
94.00	8534.0
95.00	68704.0
95.90	4770.0
96.90	108.0
103.90	390.0
104.70	108.0
105.70	360.0
114.70	115.0
115.80	338.0
116.90	581.0
117.80	270.0
118.80	473.0
127.80	431.0
128.80	125.0
129.90	294.0
130.70	126.0
134.80	177.0
140.80	826.0
142.90	1084.0
144.80	135.0
147.80	290.0
154.80	197.0
156.90	109.0
158.90	123.0
171.90	542.0
173.90	57328.0
174.90	4353.0
175.90	54992.0
176.90	3704.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
36.00	616.0
36.90	2775.0
38.00	2487.0
39.00	986.0
44.00	481.0
44.90	491.0
47.00	577.0
47.80	324.0
49.00	2810.0
50.00	11609.0
51.00	3421.0
51.90	127.0
54.90	244.0
56.00	1029.0
57.00	1639.0
59.90	530.0
61.00	3440.0
62.00	3476.0
63.00	2607.0
63.90	331.0
64.90	383.0
68.00	7022.0
69.00	7070.0
69.90	474.0
71.90	464.0
73.00	3270.0
74.00	12729.0
75.00	38232.0
76.00	3207.0
77.00	306.0
78.10	209.0
78.90	2629.0
79.90	863.0
80.90	2483.0
81.80	614.0
86.80	2316.0
87.90	2081.0
90.90	299.0
92.00	2218.0
93.00	3432.0
94.00	8495.0
95.00	68536.0
95.90	4692.0
97.00	112.0
103.80	407.0
104.80	125.0
105.70	385.0
114.80	106.0
115.80	325.0
116.90	627.0
117.70	273.0
118.80	539.0
127.80	310.0
128.90	112.0
129.90	325.0
130.80	132.0
134.80	179.0
140.80	892.0
142.90	1140.0
144.90	147.0
147.80	226.0
154.80	235.0
157.00	129.0
158.90	105.0
160.70	111.0
171.90	612.0
172.90	554.0
173.90	58064.0
174.90	4149.0
175.90	55816.0
176.90	3748.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057