
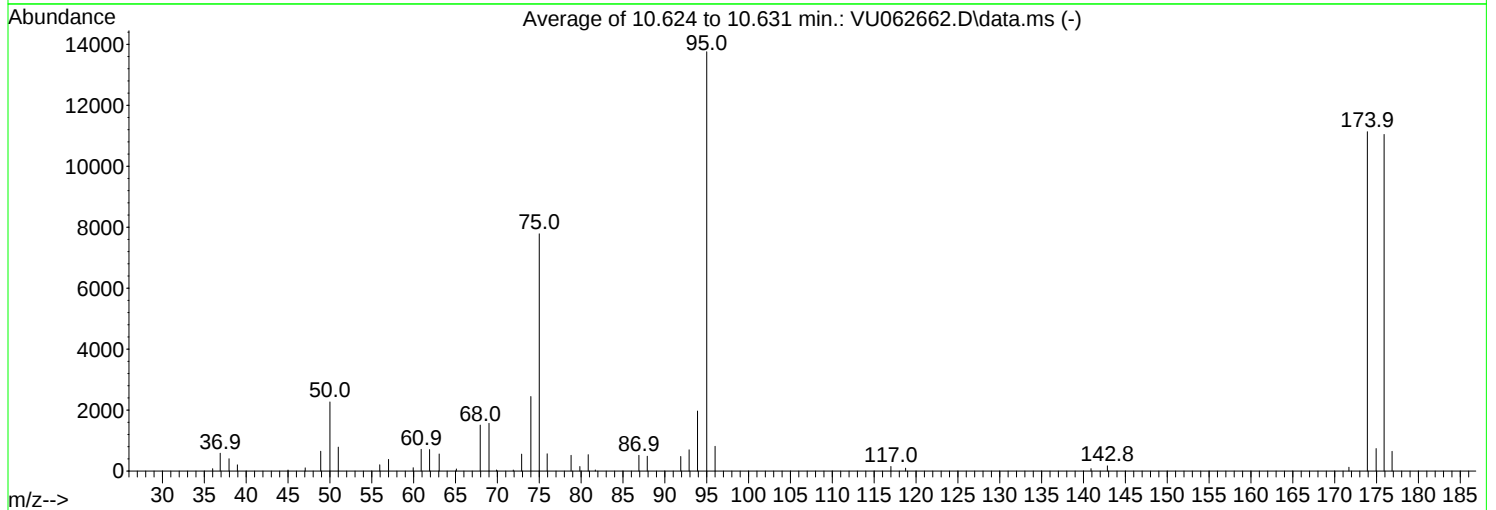


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010825\
Data File : VU062662.D
Acq On : 08 Jan 2025 09:07
Operator : MD/SY
Sample : BFB082
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB082

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010825WMA.M
Title : VOC Analysis
Last Update : Wed Jan 08 23:36:50 2025

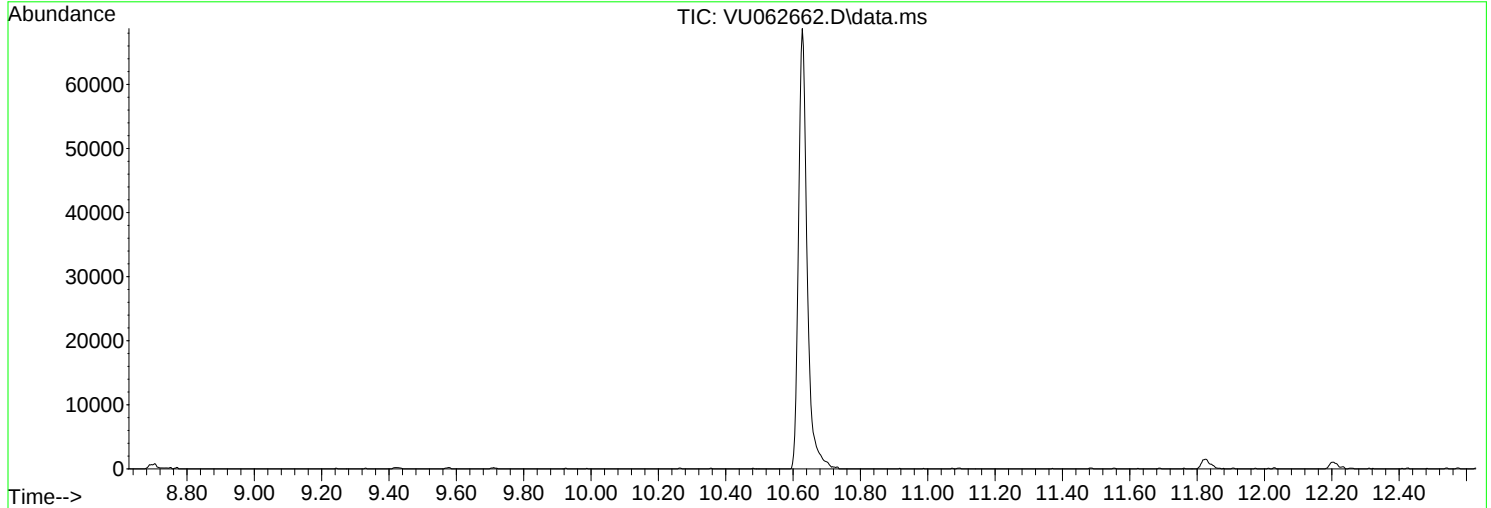

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2893

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	2267	PASS
75	95	30	80	56.6	7784	PASS
95	95	100	100	100.0	13757	PASS
96	95	5	9	5.9	813	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.9	11134	PASS
175	174	5	9	6.6	739	PASS
176	174	95	101	99.2	11043	PASS
177	176	5	9	5.9	647	PASS

Scan 2903 (10.624 min): VU062662.D\data.ms
BFB082
m/z Abundance

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
36.00	123.0
36.90	561.0
38.00	385.0
39.00	232.0
48.90	599.0
50.00	2302.0
51.00	751.0
56.00	196.0
57.00	308.0
60.00	110.0
60.90	758.0
61.90	718.0
63.10	632.0
67.90	1501.0
69.00	1522.0
71.90	101.0
72.90	538.0
74.00	2449.0
75.00	7751.0
75.90	509.0
78.80	477.0
79.90	148.0
80.80	543.0
81.70	109.0
86.90	518.0
87.90	498.0
91.90	507.0
92.90	730.0
93.90	1869.0
95.00	13563.0
96.00	742.0
117.00	155.0
140.90	134.0
142.80	170.0
171.70	136.0
173.90	10722.0
175.00	740.0
175.90	10451.0
176.80	623.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
36.00	110.0
36.90	599.0
37.90	417.0
39.00	212.0
47.10	140.0
48.90	692.0
50.00	2324.0
51.00	824.0
55.90	217.0
57.00	388.0
59.90	109.0
60.90	726.0
61.90	729.0
63.10	569.0
65.10	100.0
68.00	1561.0
69.00	1636.0
72.90	570.0
74.00	2529.0
75.00	8057.0
76.00	564.0
78.80	518.0
79.90	152.0
80.90	564.0
86.90	529.0
87.90	501.0
91.90	484.0
92.90	731.0
93.90	2085.0
95.00	14225.0
96.00	824.0
117.00	163.0
118.80	134.0
140.90	106.0
142.90	182.0
171.70	136.0
173.90	11427.0
175.00	787.0
175.90	11410.0
176.90	665.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
36.90	599.0
37.90	413.0
38.90	171.0
45.00	102.0
47.00	178.0
48.90	663.0
50.00	2174.0
51.00	782.0
55.90	204.0
57.00	451.0
59.90	111.0
60.90	658.0
61.90	667.0
63.00	478.0
65.10	107.0
68.00	1463.0
69.00	1542.0
69.90	107.0
72.90	560.0
74.00	2360.0
75.00	7544.0
76.00	628.0
78.80	556.0
79.80	146.0
80.90	510.0
86.90	503.0
87.90	462.0
91.90	446.0
92.90	632.0
93.90	1955.0
95.00	13483.0
96.00	872.0
117.00	135.0
118.70	149.0
142.90	164.0
171.70	107.0
173.90	11252.0
174.90	691.0
175.90	11267.0
176.90	654.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082