

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010923\
 Data File : VU052637.D
 Acq On : 09 Jan 2023 11:38
 Operator : JC/MD
 Sample : 01036-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	41	47	66	rBV	23531	34893	2.26%	0.311%
2	1.600	73	81	103	rVB	204929	245992	15.92%	2.193%
3	1.909	170	177	206	rVB	160393	253781	16.42%	2.262%
4	2.565	369	381	395	rBV	316838	514667	33.31%	4.588%
5	2.871	474	476	479	rVB2	545	240	0.02%	0.002%
6	2.919	489	491	494	rBV2	423	234	0.02%	0.002%
7	2.944	494	499	501	rBV2	620	622	0.04%	0.006%
8	3.044	520	530	543	rBV2	5416	11192	0.72%	0.100%
9	3.350	622	625	627	rBV	329	227	0.01%	0.002%
10	3.501	669	672	674	rBV	605	416	0.03%	0.004%
11	3.514	674	676	679	rVV2	402	223	0.01%	0.002%
12	3.703	730	735	739	rBV3	454	465	0.03%	0.004%
13	3.732	739	744	747	rVV3	421	429	0.03%	0.004%
14	3.771	751	756	760	rVB2	474	529	0.03%	0.005%
15	3.803	760	766	769	rBV3	560	597	0.04%	0.005%
16	3.944	807	810	816	rVB3	271	260	0.02%	0.002%
17	4.215	891	894	897	rVB3	357	270	0.02%	0.002%
18	4.292	915	918	923	rBV3	425	372	0.02%	0.003%
19	4.395	948	950	955	rVB3	395	287	0.02%	0.003%
20	4.420	955	958	960	rVV	314	254	0.02%	0.002%
21	4.472	971	974	978	rVB	355	302	0.02%	0.003%
22	4.514	984	987	991	rVB3	273	215	0.01%	0.002%
23	4.536	991	994	997	rVB2	465	240	0.02%	0.002%
24	4.623	1006	1021	1066	rBV	129897	364429	23.59%	3.249%
25	4.967	1123	1128	1131	rBV	522	405	0.03%	0.004%
26	5.060	1139	1157	1180	rBV	272762	603098	39.03%	5.376%
27	5.198	1196	1200	1204	rVB4	509	368	0.02%	0.003%
28	5.282	1219	1226	1230	rBV5	802	1167	0.08%	0.010%
29	5.333	1237	1242	1244	rBV4	663	588	0.04%	0.005%
30	5.362	1244	1251	1252	rBV3	896	774	0.05%	0.007%
31	5.481	1285	1288	1293	rVB3	482	391	0.03%	0.003%
32	5.549	1306	1309	1312	rBV2	253	237	0.02%	0.002%
33	5.587	1318	1321	1326	rVB3	304	290	0.02%	0.003%
34	5.719	1339	1362	1395	rBV2	565383	1545153	100.00%	13.774%
35	5.954	1432	1435	1437	rVB2	343	206	0.01%	0.002%
36	6.034	1456	1460	1466	rVB4	610	590	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010923\
 Data File : VU052637.D
 Acq On : 09 Jan 2023 11:38
 Operator : JC/MD
 Sample : 01036-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

37	6.105	1477	1482	1486	rBV3	355	368	0.02%	0.003%
38	6.128	1486	1489	1491	rVV2	495	281	0.02%	0.003%
39	6.247	1511	1526	1550	rVV	416259	800473	51.81%	7.135%
40	6.333	1550	1553	1556	rVV2	847	681	0.04%	0.006%
41	6.349	1556	1558	1562	rVV3	889	548	0.04%	0.005%
42	6.517	1607	1610	1619	rBV5	1165	1746	0.11%	0.016%
43	6.571	1624	1627	1629	rBV	322	218	0.01%	0.002%
44	6.604	1633	1637	1642	rBV3	486	483	0.03%	0.004%
45	6.687	1648	1663	1685	rBV	380408	735078	47.57%	6.553%
46	6.813	1700	1702	1706	rVB2	631	351	0.02%	0.003%
47	6.848	1709	1713	1717	rBV4	290	336	0.02%	0.003%
48	6.948	1740	1744	1749	rBV2	334	371	0.02%	0.003%
49	7.034	1762	1771	1773	rBV3	419	592	0.04%	0.005%
50	7.092	1785	1789	1793	rBV3	296	225	0.01%	0.002%
51	7.179	1810	1816	1817	rBV4	1305	1084	0.07%	0.010%
52	7.259	1840	1841	1846	rVB2	420	253	0.02%	0.002%
53	7.288	1847	1850	1853	rVB2	325	213	0.01%	0.002%
54	7.375	1873	1877	1878	rBV	393	265	0.02%	0.002%
55	7.439	1894	1897	1901	rBV2	536	469	0.03%	0.004%
56	7.507	1915	1918	1922	rBV2	340	326	0.02%	0.003%
57	7.562	1922	1935	1962	rVV	185092	330734	21.40%	2.948%
58	7.690	1969	1975	1983	rVB5	639	1105	0.07%	0.010%
59	7.790	2003	2006	2009	rBV	321	261	0.02%	0.002%
60	7.896	2023	2039	2072	rBV	636327	1097605	71.04%	9.784%
61	8.041	2079	2084	2087	rBV5	618	485	0.03%	0.004%
62	8.124	2106	2110	2113	rVB2	617	495	0.03%	0.004%
63	8.176	2113	2126	2142	rBV2	135564	228506	14.79%	2.037%
64	8.404	2193	2197	2198	rBV4	351	290	0.02%	0.003%
65	8.436	2206	2207	2212	rVB	324	191	0.01%	0.002%
66	8.465	2212	2216	2220	rBV3	529	502	0.03%	0.004%
67	8.523	2230	2234	2235	rBV2	391	311	0.02%	0.003%
68	8.639	2256	2270	2303	rBV2	391895	796496	51.55%	7.100%
69	8.909	2352	2354	2356	rBV	357	191	0.01%	0.002%
70	8.989	2377	2379	2384	rVB2	568	438	0.03%	0.004%
71	9.015	2384	2387	2390	rBV3	329	186	0.01%	0.002%
72	9.121	2416	2420	2422	rVV2	324	287	0.02%	0.003%
73	9.266	2459	2465	2471	rBV3	380	501	0.03%	0.004%
74	9.295	2471	2474	2477	rBV	320	190	0.01%	0.002%
75	9.317	2477	2481	2485	rBV2	475	405	0.03%	0.004%
76	9.346	2488	2490	2494	rVB3	424	191	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010923\
 Data File : VU052637.D
 Acq On : 09 Jan 2023 11:38
 Operator : JC/MD
 Sample : 01036-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

77	9.414	2495	2511	2533	rBV	611403	996699	64.50%	8.885%
78	9.652	2582	2585	2590	rVB3	516	409	0.03%	0.004%
79	9.684	2592	2595	2596	rBV3	427	236	0.02%	0.002%
80	9.697	2597	2599	2602	rVB2	512	319	0.02%	0.003%
81	9.954	2676	2679	2682	rBV2	355	248	0.02%	0.002%
82	10.095	2719	2723	2724	rBV4	424	272	0.02%	0.002%
83	10.147	2736	2739	2743	rVB2	286	258	0.02%	0.002%
84	10.291	2781	2784	2791	rBV3	332	365	0.02%	0.003%
85	10.336	2792	2798	2803	rBV2	393	569	0.04%	0.005%
86	10.394	2813	2816	2818	rBV2	371	258	0.02%	0.002%
87	10.427	2823	2826	2831	rBV2	384	450	0.03%	0.004%
88	10.523	2851	2856	2858	rBV3	415	299	0.02%	0.003%
89	10.587	2874	2876	2879	rVB2	451	269	0.02%	0.002%
90	10.697	2906	2910	2912	rBV2	319	289	0.02%	0.003%
91	10.754	2914	2928	2944	rVV	487852	785707	50.85%	7.004%
92	11.021	3009	3011	3014	rVV	340	190	0.01%	0.002%
93	11.163	3052	3055	3062	rVB3	379	418	0.03%	0.004%
94	11.198	3062	3066	3069	rBV3	292	287	0.02%	0.003%
95	11.394	3122	3127	3132	rBV4	454	601	0.04%	0.005%
96	11.436	3138	3140	3143	rVB	361	190	0.01%	0.002%
97	11.645	3202	3205	3207	rBV2	407	309	0.02%	0.003%
98	11.742	3230	3235	3239	rBV4	554	579	0.04%	0.005%
99	11.809	3243	3256	3281	rVV	563144	883094	57.15%	7.872%
100	12.188	3361	3374	3391	rBV	601899	957828	61.99%	8.538%



Sum of corrected areas: 11218277

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010923\
Data File : VU052637.D
Acq On : 09 Jan 2023 11:38
Operator : JC/MD
Sample : 01036-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

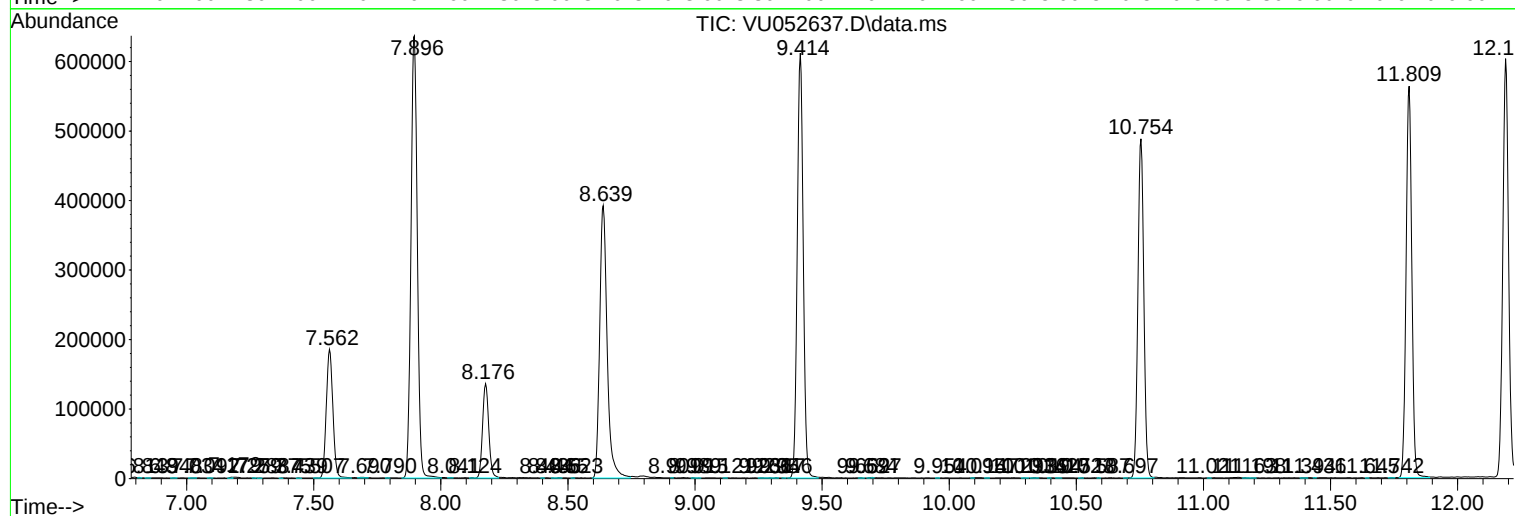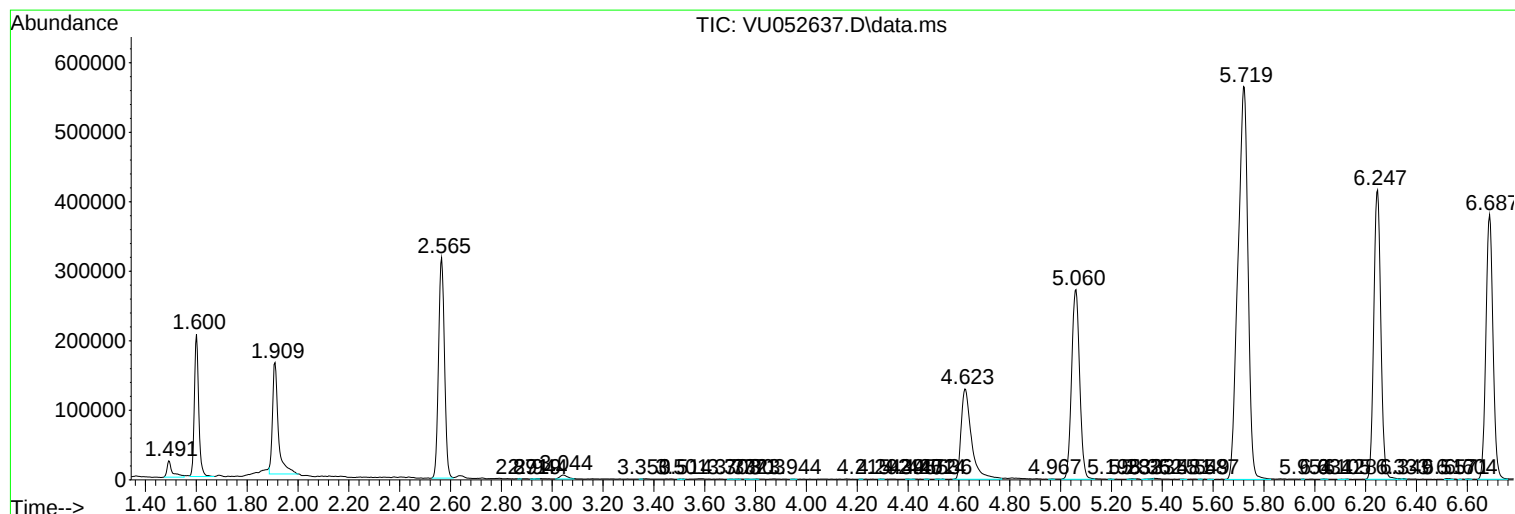

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010923\
Data File : VU052637.D
Acq On : 09 Jan 2023 11:38
Operator : JC/MD
Sample : 01036-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010923\
Data File : VU052637.D
Acq On : 09 Jan 2023 11:38
Operator : JC/MD
Sample : 01036-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc